



**memmert**  
Experts in Thermostatics

UNxx UFxx  
INxx IFxx



## OPERATING INSTRUCTIONS

UNIVERSAL OVEN U  
INCUBATOR I

100% ATMOSAFE. MADE IN GERMANY.

[www.memmert.com](http://www.memmert.com) | [www.atmosafe.net](http://www.atmosafe.net)

## Manufacturer and customer service

Memmert GmbH + Co. KG  
Willi-Memmert-Straße 90–96  
D-91186 Büchenbach  
Deutschland

Phone: +49 (0)9122 925-0  
Fax: +49 (0)9122 14585  
E-mail: [sales@memmert.com](mailto:sales@memmert.com)  
Internet: [www.memmert.com](http://www.memmert.com)

### Customer service:

Service hotline: +49 (0)9171 9792 911  
Service fax: +49 (0)9171 9792 979  
E-mail: [service@memmert.com](mailto:service@memmert.com)

When contacting customer service, always quote the product serial number on the nameplate (see page 12).

### Shipping address for repairs:

Memmert GmbH + Co. KG  
Kundenservice  
Willi-Memmert-Str. 90-96  
DE-91186 Büchenbach  
Germany

Please contact our customer service before sending appliances for repair or before returning equipment, otherwise, we have to refuse acceptance of the shipment.

© 2016 MEMMERT GmbH + Co. KG

D33363 | Date 06/2016

We reserve the right to make changes

## About this manual

---

### Purpose and target group

This manual describes the construction, function, transport and operation of the universal ovens UNxx/UFxx and the incubators INxx/IFxx. It is intended for use by trained personnel of the owner who have the task of operating and/or maintaining the respective appliance.

If you are asked to work on the appliance, read this manual carefully before starting. Familiarise yourself with the safety regulations. Only perform work that is described in this manual. If there is something you do not understand, or certain information is missing, ask your superior or contact the manufacturer. Do not do anything without authorisation.

### Versions

The appliances are available in different configurations and sizes. If specific equipment features or functions are available only for certain configurations, this is indicated at the relevant points in this manual.

The functions described in this manual refer to the latest firmware version.

Due to individual configurations and sizes, illustrations in this manual may be slightly different from the actual appearance. Function and operation are identical.

### Other documents that have to be observed:

- ▶ For operation of the appliance with MEMMERT AtmoCONTROL, observe the separate software manual
- ▶ For service and repair (see page 44), please refer to the separate service manual

### Storage and forwarding

This instruction manual belongs with the appliance and should always be stored where persons working on the appliance have access to it. It is the responsibility of the owner to ensure that persons who are working or will work on the appliance are informed as to the whereabouts of this instruction manual. We recommend that it is always stored in a protected location close to the appliance. Make sure that the instruction manual is not damaged by heat or humidity. If the appliance is sold on or transported and then set up again at a different location, the operating instructions must go with it.

You will find the current version of our operating manual as pdf file if you go to [www.memmert.com/de/service/downloads/bedienungsanleitung/](http://www.memmert.com/de/service/downloads/bedienungsanleitung/).

# Contents

<b>1. For your Safety</b>	<b>6</b>
1.1 Terms and signs used.....	6
1.1.1 Terms used .....	6
1.1.2 Signs used .....	6
1.2 Product safety and dangers .....	7
1.3 Requirements of the operating personnel .....	7
1.4 Responsibility of the owner .....	8
1.5 Intended use .....	8
1.6 Changes and alterations .....	8
1.7 Behaviour in case of malfunctions and irregularities .....	9
1.8 Switching off the appliance in an emergency .....	9
<b>2. Construction and description</b>	<b>10</b>
2.1 Construction .....	10
2.2 Function .....	11
2.3 Material .....	11
2.4 Electrical equipment .....	11
2.5 Connections and interfaces .....	12
2.5.1 Electrical connection .....	12
2.5.2 Communication interface .....	12
2.6 Designation (nameplate) .....	12
2.7 Technical data .....	13
2.8 Applied directives and standards .....	14
2.9 Declaration of conformity .....	14
2.10 Ambient conditions .....	15
2.11 Scope of delivery .....	15
2.12 Optional accessories .....	15
<b>3. Delivery, transport and setting up</b>	<b>16</b>
3.1 For your Safety .....	16
3.2 Delivery .....	17
3.3 Transport .....	17
3.4 Unpacking .....	17
3.4.1 Checking for completeness and transport damage .....	17
3.4.2 Removing the transport protection .....	17
3.4.3 Disposing of packaging material .....	17
3.5 Storage after delivery .....	17
3.6 Setting up .....	18
3.6.1 Prerequisites .....	18
3.6.2 Installation options .....	19
3.6.3 Tilt protection .....	20
3.6.4 Adjusting the doors (only for model sizes 450 and 750) .....	21
<b>4. Putting into operation</b>	<b>22</b>
4.1 Connecting the appliance .....	22
4.2 Switching on .....	22

<b>5. Operation and control</b>	<b>23</b>
5.1 Operating personnel.....	23
5.2 Opening the door.....	23
5.3 Loading the appliance.....	24
5.4 Operating the appliance.....	24
5.4.1 ControlCOCKPIT .....	24
5.4.2 Basic operation.....	26
5.4.3 Operating modes .....	26
5.4.4 Manual mode.....	27
5.4.5 Operation with digital backwards counter with target time setting, adjustable from 1 minute to 99 days (Timer).....	27
5.5 Temperature monitoring .....	28
5.5.1 Electronic temperature monitoring .....	29
5.5.2 Mechanical temperature monitoring: Temperature limiter (TB).....	30
5.5.3 Function .....	30
5.6 Ending operation.....	30
<b>6. Malfunctions, warning and error messages</b>	<b>31</b>
6.1 Warning messages of the temperature monitoring function .....	31
6.2 Malfunctions, operating problems and appliance errors .....	32
6.3 Power failure.....	33
<b>7. Menu mode</b>	<b>34</b>
7.1 Overview.....	34
7.2 Basic operation in menu mode using the example of language selection.....	35
7.3 Setup.....	36
7.3.1 IP address and subnet mask .....	36
7.3.2 Unit.....	37
7.3.3 Temperature monitoring (Alarm Temp and Max Alarm) .....	37
7.3.4 Timer Mode.....	39
7.3.5 Type of the slide-in unit (Grid or Shelf) .....	39
7.3.6 Remote control .....	39
7.3.7 Gateway.....	40
7.4 Date and Time .....	40
7.5 Calibration .....	42
<b>8. Maintenance and service</b>	<b>44</b>
8.1 Cleaning.....	44
8.1.1 Working chamber and metal surfaces.....	44
8.1.2 Plastic parts .....	44
8.1.3 Glass surfaces.....	44
8.2 Regular maintenance.....	44
8.3 Repairs and service .....	44
<b>9. Storage and disposal</b>	<b>45</b>
9.1 Storage .....	45
9.2 Disposal .....	45
<b>Index</b>	<b>46</b>

# 1. For your Safety

## 1.1 Terms and signs used















In this manual and on the appliance itself, certain common terms and signs are used to warn you of possible dangers or to give you hints that are important in avoiding injury or damage. Observe and follow these hints and regulations to avoid accidents and damage. These terms and signs are explained below.

### 1.1.1 Terms used

**"Warning"** is used whenever you or somebody else could be injured if you do not observe the accompanying safety regulation.

**"Caution"** is used for information that is important for avoiding damage.

### 1.1.2 Signs used


Warning signs (warning of a danger)					
					
Danger of electrocution	Danger of explosion	Dangerous gases / vapours	Danger of burns	Danger of toppling over	Hazard area! Observe the operating instructions
Prohibition signs (forbidding an action)					
					
Do not lift	Do not tilt	Do not enter			
Regulation signs (stipulating an action)					
					
Disconnect the mains plug	Wear gloves	Wear safety boots	Observe information in separate manual		
Other icons					
	Important or useful additional information				

## 1.2 Product safety and dangers

The appliances described in this manual are technically sophisticated, manufactured using high-quality materials and subject to many hours of testing in the factory. They contain the latest technology and comply with recognised technical safety regulations. However, there are still risks involved, even when the appliances are used as intended. These are described below.

**Warning!**

After removing covers, live parts may be exposed. You may receive an electric shock if you touch these parts. Disconnect the mains plug before removing any covers. Only electrical technicians may work on the electrical equipment of the appliances.

**Warning!**

When loading the appliance with an unsuitable load, poisonous or explosive vapours or gases may be produced. This could cause the appliance to explode, and persons could be severely injured or poisoned. The appliance may only be loaded with materials/test objects which do not form any toxic or explosive vapours when heated up (see also Intended use on page 8).

**Warning!**

If the door is open while the appliance is in operation, the appliance may overheat and pose a fire hazard. Do not leave the door open during operation.

**Warning!**

Depending on operation, the surfaces in the working chamber and the chamber load may still be very hot after the appliance is switched off. Touching these surfaces can cause burns. Wear heat-resistant protective gloves or wait until the appliance cools down.

**Warning!**

In case of appliances of a certain size, you can get accidentally locked in, which is life-threatening. Do not climb into the appliance!

## 1.3 Requirements of the operating personnel

The appliance may only be operated and maintained by persons who are of legal age and have been instructed accordingly. Personnel who are to be trained, instructed or who are undergoing general training may only work with the appliance under the continuous supervision of an experienced person.

Repairs may only be performed by qualified electricians. The regulations in the separate service manual must be observed.



## 1.4 Responsibility of the owner

The owner of the appliance

- ▶ is responsible for the flawless condition of the appliance and for its proper operation in accordance with its intended use (see page 8);
- ▶ is responsible for ensuring that persons who are to operate or service the appliance are qualified to do this, have been instructed accordingly and are familiar with the operating instructions at hand;
- ▶ must know about the applicable guidelines, requirements and operational safety regulations, and train staff accordingly;
- ▶ is responsible for ensuring that unauthorised persons have no access to the appliance;
- ▶ is responsible for ensuring that the maintenance plan is adhered to and that maintenance work is carried out properly (see page 44);
- ▶ has to ensure that the appliance and its surroundings are kept clean and tidy, for example through corresponding instructions and inspections;
- ▶ is responsible for ensuring that personal protective clothing is worn by operating personnel, e.g. work clothes, safety shoes and protective gloves.

## 1.5 Intended use

This appliance is exclusively intended for heating up non-explosive substances and objects. Any other use is improper, and may result in hazards and damage.

The appliance is not explosion-proof (does not comply with the German workplace health & safety regulation VBG 24). The appliance may only be loaded with materials and substances which cannot form any toxic or explosive vapours at the set temperature and which cannot explode, burst or ignite.

The appliance may not be used for drying, vaporising and branding paints or similar materials the solvents of which could form an explosive mixture when combined with air. If there is any doubt as to the composition of materials, they must not be loaded into the appliance. Potentially explosive gas-air mixtures must not form, neither in the working chamber nor in the direct vicinity of the appliance.

### Appliances IFxx/UFxx for use as medical device

For appliances IFxx and UFxx with extended overtemperature protection (option A6, recognisable due to standard DIN 12880-2007-Kl.:3.1 on the nameplate) subject to the 93/42/EEC directive (Directive of the council on harmonisation of the laws of the member states relating to medical devices), the intended use is defined as follows: The appliance's intended use is the warming of non-sterile cloths and covers.

## 1.6 Changes and alterations

No unauthorised changes or alterations may be made to the appliance. No parts may be added or inserted which have not been approved by the manufacturer.

Unauthorised modifications or changes result in the CE declaration of conformity losing its validity and the appliance must no longer be operated.

The manufacturer is not liable for any damage, danger or injuries that result from unauthorised changes or alterations, or from non-observance of the regulations in this manual.



## 1.7 Behaviour in case of malfunctions and irregularities

The appliance may only be used in a flawless condition. If you as the operator notice irregularities, malfunctions or damage, immediately take the appliance out of service and inform your superior.


**i** You can find information on correcting malfunctions from page 31.

## 1.8 Switching off the appliance in an emergency

Push the On/Off switch on the control panel (Fig. 1) and disconnect power plug. This disconnects the appliance from the power supply at all poles.



**Warning!**  
Depending on the operation performed, the surfaces in the working chamber and the chamber load may still be very hot after the appliance is switched off. Touching these surfaces can cause burns. Wear heat-resistant protective gloves or wait until the appliance cools down.

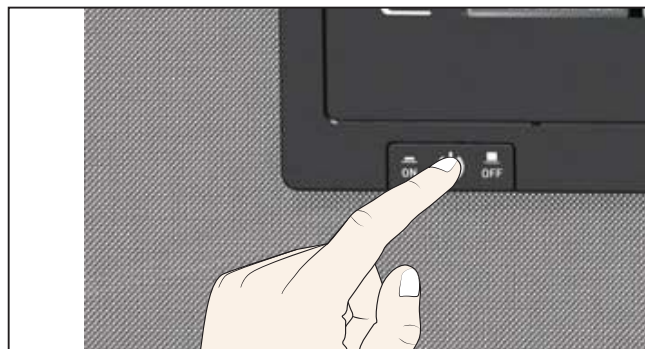

*Fig. 1*  
Switch off the appliance by pressing the On/Off switch

## 2. Construction and description

### 2.1 Construction



Fig. 2 Construction

- |  |                                      |
|--|--------------------------------------|
| 1 ControlCOCKPIT with capacitive function keys (see page 25) | 4 Steel grid                         |
| 2 On/Off switch (see page 22)                                | 5 Working chamber                    |
| 3 Working chamber fan (for UFxx/IFxx appliances only)        | 6 Nameplate (covered, see page 12)   |
|  | 7 Door handle (see page 23)          |
|  | 8 Turn control with confirmation key |

## 2.2 Function

Appliances of the UNxx and INxx type series feature natural circulation (convection). For the UFxx and IFxx type series, air is circulated by a fan at the working chamber rear panel Fig. 3, No. 1). It increases the air flow and provides stronger horizontal forced air circulation than natural convection.

In both the convection and fan ventilated appliances, supply air (2) is preheated in a pre-heating chamber (3). Through the ventilation slits in the side panel of the working chamber, the pre-heated air is introduced into the interior of the chamber. The supply and exhaust air (5) volume (air change) is controlled by the air flap (4) on the rear panel of the appliance.

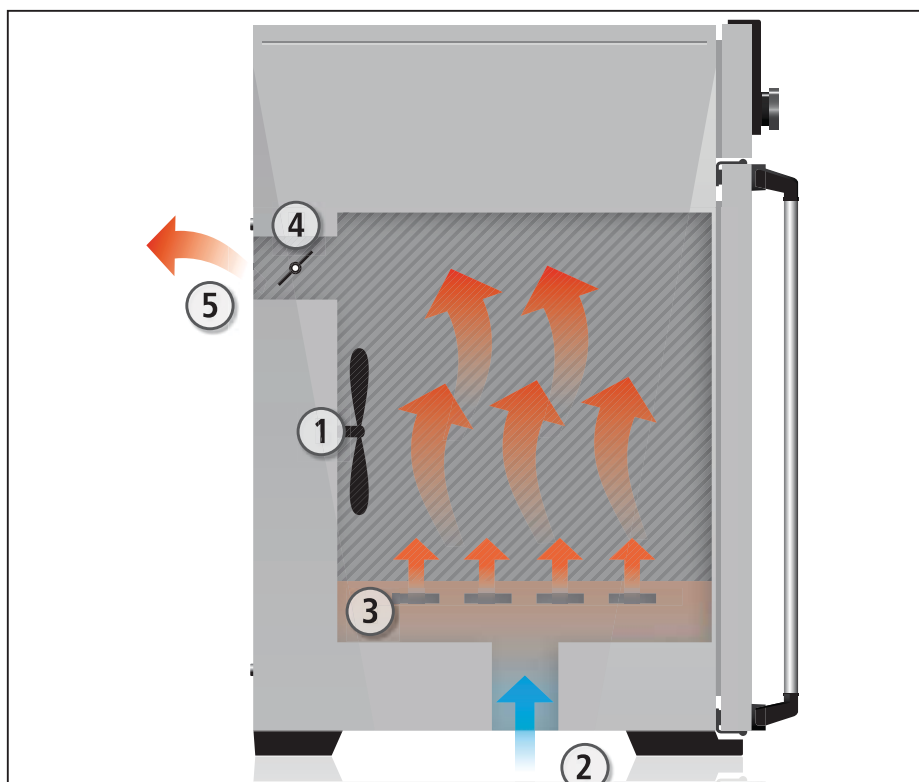


Fig. 3      *Function*  
 1   *Fan*  
 2   *Fresh air*  
 3   *Pre-heating chamber*  
 4   *Air flap*  
 5   *Exhaust air*

## 2.3 Material

For the outer housing, MEMMERT deploys stainless steel (Mat.No. 1.4016 – ASTM 430) and for the interior, stainless steel (Mat.No. 1.4301 – ASTM 304) is used, which stands out through its high stability, optimal hygienic properties and corrosion-resistance towards many (but not all!) chemical compounds (caution for example with chlorine compounds).

The chamber load for the appliance must be carefully checked for chemical compatibility with the materials mentioned. A material resistance table can be requested from the manufacturer.

## 2.4 Electrical equipment

- ▶ Operating voltage and current consumption: See nameplate
- ▶ Protection class I, i.e. operating insulation with PE conductor in accordance with EN 61010
- ▶ Protection type IP 20 acc. to EN 60 529
- ▶ Interference suppression acc. to EN 55011 class B
- ▶ Appliance fuse: Fusible link 250 V/15 A quick-blow
- ▶ The temperature controller is protected with a miniature fuse 100 mA (160 mA at 115 V)

## 2.5 Connections and interfaces

### 2.5.1 Electrical connection

This appliance is intended for operation on an electrical power system with a system impedance  $Z_{\max}$  of a maximum of 0.292 ohm at the point of transfer (service line). The operator must ensure that the appliance is operated only on an electrical power system that meets these requirements. If necessary, you can ask your local energy supply company what the system impedance is.

Observe the country-specific regulations when connecting (e.g. in Germany DIN VDE 0100 with residual current circuit breaker).

### 2.5.2 Communication interface

The Ethernet interface is intended for appliances which meet the requirements of IEC 60950-1.

Via Ethernet interface, the appliance can be connected to a network to read out protocol logs with AtmoCONTROL, the optional appliance software. The Ethernet interface is located on the rear of the appliance (Fig. 4).

For identification purposes, each appliance connected must have its own unique IP address. Setting the IP address is described on page 36.

With an optional USB to Ethernet converter, the appliance can be directly connected to a computer / laptop (see Optional accessories on page 15).

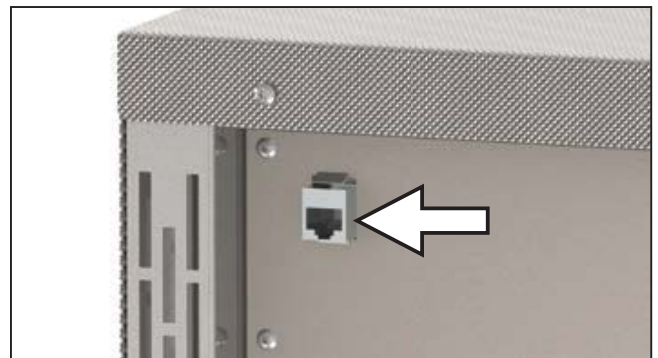


Fig. 4 Ethernet interface

## 2.6 Designation (nameplate)

The nameplate (Fig. 5) provides information about the appliance model, manufacturer and technical data. It is attached to the front of the appliance, on the right side under the door (see page 10).

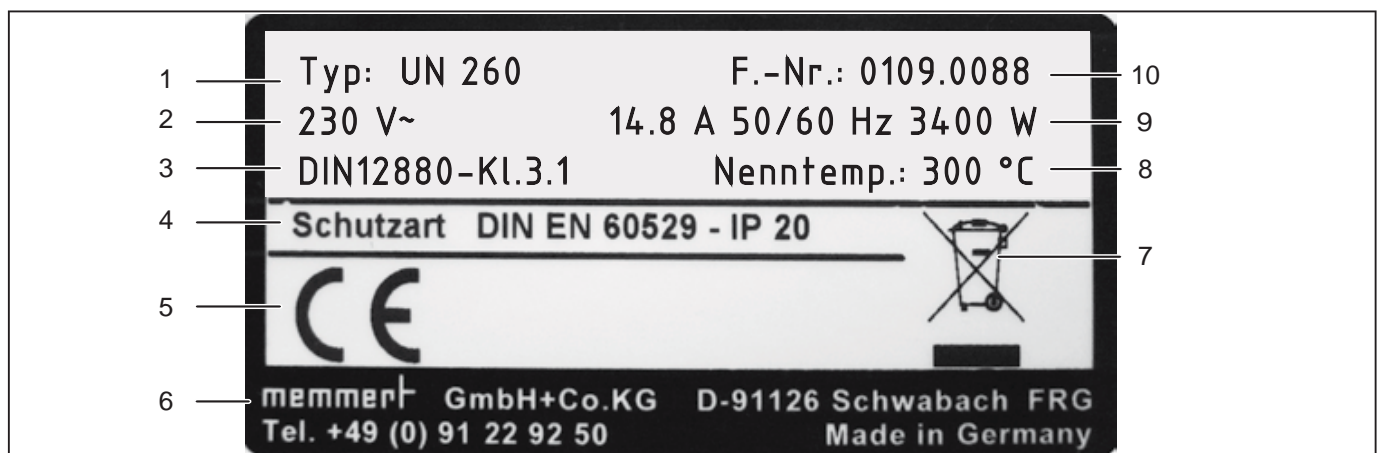


Fig. 5 Nameplate (example)

- |   |                   |    |                            |
|---|-------------------|----|----------------------------|
| 1 | Type designation  | 6  | Address of manufacturer    |
| 2 | Operating voltage | 7  | Disposal note              |
| 3 | Applied standard  | 8  | Temperature range          |
| 4 | Protection type   | 9  | Connection / power ratings |
| 5 | CE conformity     | 10 | Appliance number           |

## 2.7 Technical data

Appliance size	30	55	75	110	160	260	450	750	1060
Appliance width D <sup>1</sup> [mm]	585	585	585	745	745	824	1224	1224	1224
Appliance height E <sup>1</sup> [mm]	707	787	947	867	1107	1186	1247	1726	1726
Appliance depth G <sup>1</sup> (footprint) [mm]	434	514	514	584	584	684	784	784	1035
Depth of door lock [mm]	56								
Appliance depth F <sup>1</sup> (including door handle) [mm]	490	570	570	640	640	740	840	840	1091
Working chamber width A <sup>1</sup> [mm]	400	400	400	560	560	640	1040	1040	1040
Working chamber height B <sup>1</sup> [mm]	320	400	560	480	720	800	1200	1200	1200
Working chamber depth C <sup>1</sup> [mm]	250	330	330	400	400	500	600	600	850
Chamber volume [litres]	32	53	74	108	161	256	449	749	1060
Weight [kg]	48	57	66	78	96	110	170	217	416
Power [W]	IN/IF	115 V, 50/60 Hz							
		1600	850	1100	1100	1100	1500	1800	-
	UN/UF	230 V, 50/60 Hz							
		1600	1000	1250	1400	1600	1800	2000	-
Current consumption [A]	IN/IF	230 V, 50/60 Hz							
		1600	2000	2500	2800	3200	3400	-	-
	UN/UF	115 V, 50/60 Hz							
		1600	1700	2200	2200	2200	-	-	-
max. number of sliding shelves	IN/IF	400 V, 50/60 Hz							
		7,0	4,3	5,4	6,1	7,0	7,4	7,8	8,7
	UN/UF	230 V, 50/60 Hz							
		13,9	7,4	9,6	9,6	9,6	13,0	15,7	-
max. load per sliding shelf [kg]	IN/IF	230 V, 50/60 Hz							
		7,0	8,7	10,9	12,2	13,9	14,8	-	-
	UN/UF	115 V, 50/60 Hz							
		13,9	14,8	19,1	19,1	19,1	19,1	-	-
max. load per appliance [kg]	IN/IF	400 V, 50/60 Hz							
		3	4	6	5	8	9	8	14
	UN/UF								
		60	80	120	175	210	300	300	-
Setting temperature range	IN/IF								
		+20 to +80 °C <sup>3</sup>							
	UN/UF								
		+20 to +300 °C <sup>3 4</sup>							
Adjustment precision	IN/IF								
		0,1 K							
	UN/UF								
		up to 100 °C: 0.1 K, above 100 °C: 0.5 K							

<sup>1</sup> See Fig. 6 on page 14.

<sup>2</sup> 3 x 230 V without zero

<sup>3</sup> With the interior lighting on, the minimum temperature might not be reached.

<sup>4</sup> to +250 °C if your device is equipped with a glass door



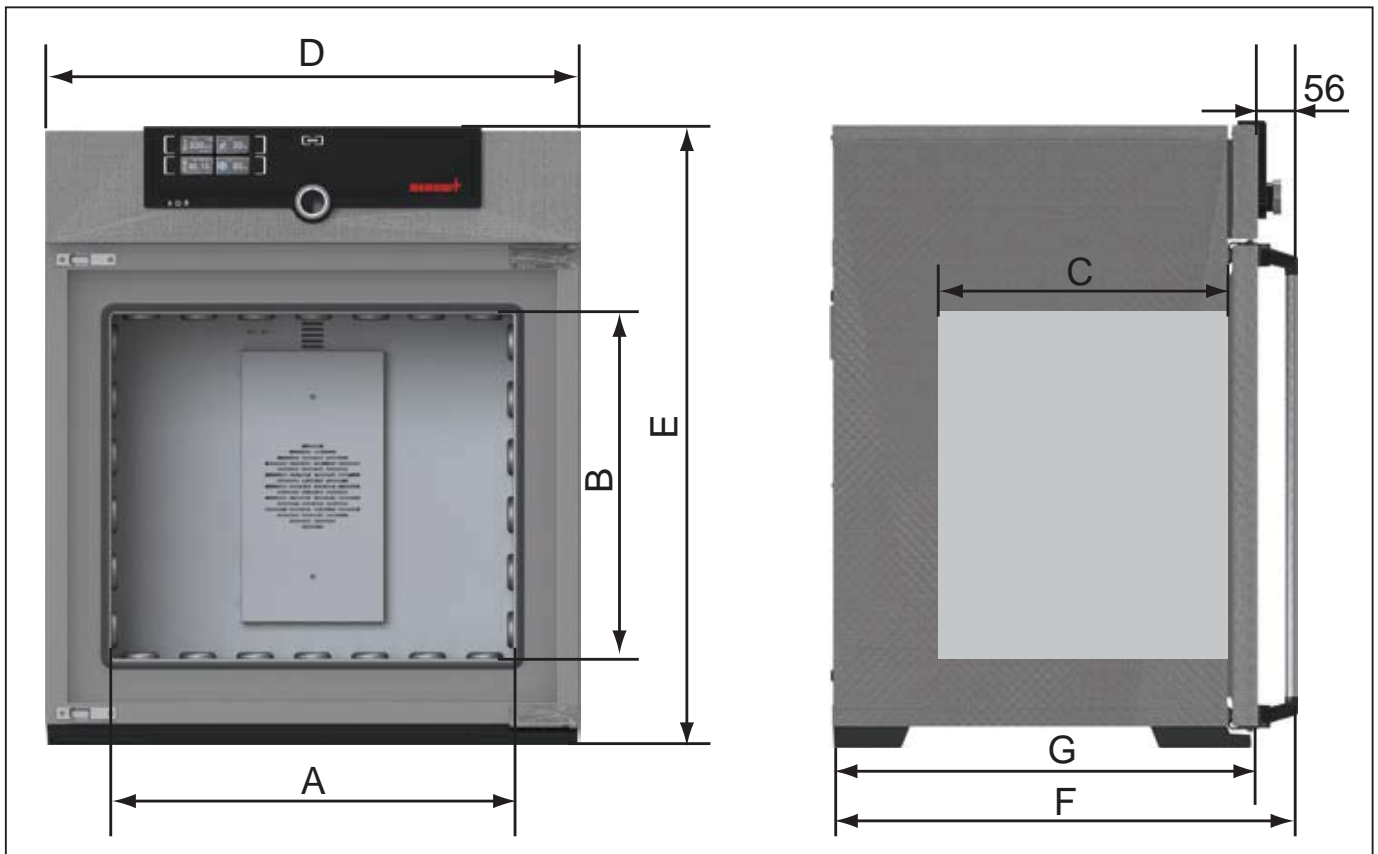


Fig. 6 Dimensions (see table on page 13)

## 2.8 Applied directives and standards

- ▶ Directive 2004/108/EC amended (Directive of the council on harmonisation of the laws of the member states on electromagnetic compatibility). Fulfilled standards:  
DIN EN 61326:2004-05, EN 61326:1997, EN 61326/A1:1998, EN 61326/A2:2001  
EN 61326/A2:2003
- ▶ Directive 2006/95/EC amended (Directive of the council on harmonisation of the laws of member states relating to electrical equipment designed for use within certain voltage limits). Standards complied with:  
DIN EN 61 010-1 (VDE 0411 Part 1)  
DIN EN 61 010-2-010 (VDE 0411 Part 2-010)  
EN 61 010-1:2001, EN 61 010-2-010

### When used as a medical device

- ▶ Directive 93/42/EEC (Directive of the Commission on the harmonisation of the legal regulations of the member states on medical devices)

## 2.9 Declaration of conformity

You can download the EC declaration of conformity of the appliance online:

English: <http://www.memmert.com/en/service/downloads/ce-statement/>

German: <http://www.memmert.com/de/service/downloads/eg-konformitaetserklaerung/>

## 2.10 Ambient conditions

- ▶ The appliance may only be used in enclosed rooms and under the following ambient conditions:

Ambient temperature	+5 °C to +40 °C
Humidity rh	max. 80 %, non-condensing
Overvoltage category	II
Pollution degree	2
Altitude of installation	max. 2,000 m above sea level

- ▶ The appliance may not be used in areas where there is a risk of explosion. The ambient air must not contain any explosive dusts, gases, vapours or gas-air mixtures. The appliance is not explosion-proof.
- ▶ Heavy dust production or aggressive vapours in the vicinity of the appliance could lead to sedimentation in the interior and, as a consequence, could result in short circuits or damage to electrical parts. For this reason, sufficient measures to prevent large clouds of dust or aggressive vapours from developing should be taken.

## 2.11 Scope of delivery

- ▶ Power cable
- ▶ Tilt protection
- ▶ One or two sliding steel grids (load capacity 30 kg each)
- ▶ The operating instructions at hand
- ▶ Calibration certificate

## 2.12 Optional accessories

- ▶ AtmoCONTROL software for reading out and processing of protocol log files
- ▶ USB to Ethernet converter (Fig. 7). Makes it possible to connect the appliance's network interface (see page 12) to the USB port of a computer / laptop.
- ▶ Reinforced, sliding steel grids with a load capacity of 60 kg each (for appliance size 110 and larger)

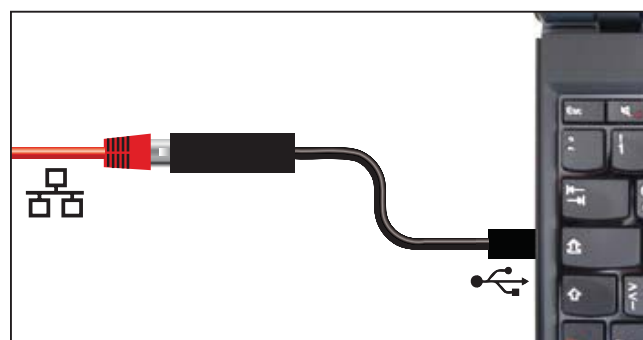


Fig. 7 Converter USB to Ethernet



### 3. Delivery, transport and setting up

#### 3.1 For your Safety



##### Warning!

Because of the heavy weight of the appliance, you could injure yourself if you try to lift it. To carry appliances of the sizes 30 and 55, at least two persons, for appliances of the sizes 75, 110, 160 and 260, four people are needed. Appliances larger than that may not be carried but must be transported with a manual pallet jack or forklift truck.

30	55	75	110	160	260	450	750



##### Warning!

You may get your hands or feet squashed when transporting and installing the appliance. Wear protective gloves and safety boots. When grasping the bottom of the appliance, grasp it only on the sides:



##### Warning!

The appliance could fall over and seriously injure you. Never tilt the appliance and transport it in upright position and without load only (except for standard accessories such as steel grids or shelves). Appliances with castors always have to be moved by two people.

## 3.2 Delivery


The appliance is packed in cardboard and is delivered on a wooden pallet.

## 3.3 Transport

The appliance can be transported in three ways:

- ▶ With a forklift truck; move the forks of the truck entirely under the pallet
- ▶ On a manual pallet jack
- ▶ On its own castors, in case of the corresponding configuration, for which the catch on the (front) castors must be released

## 3.4 Unpacking

 To avoid damage, do not unpack the appliance until you reach the installation site.

Remove the cardboard packaging by pulling it upwards or carefully cutting along an edge.

### 3.4.1 Checking for completeness and transport damage

- ▶ Check the delivery note to ensure that the delivery is complete.
- ▶ Check the appliance for damage.

If you notice deviations from the delivery note, damage or irregularities, do not put the appliance into operation but inform the haulage company and the manufacturer.

### 3.4.2 Removing the transport protection

Remove the transport protection. It is located between the door hinge, door and frame and has to be removed after opening the door.

### 3.4.3 Disposing of packaging material

Dispose of the packaging material (cardboard, wood, foil) in accordance with the applicable disposal regulations for the respective material in your country.

## 3.5 Storage after delivery

If the appliance is first to be stored after delivery: Read the storage conditions from page 45.

### 3.6 Setting up

**Warning!**

Due to its centre of gravity, the appliance can fall over to the front and injure you or other people. Always attach the appliance to a wall with the tilt protection (see page 20). If this cannot be done due to space problems, do not operate the appliance and do not open the door. Contact the Memmert service team (see page 2).

#### 3.6.1 Prerequisites

The installation site must be flat and horizontal and must be able to reliably bear the weight of the appliance (see Technical data on page 13). Do not place the appliance on a flammable surface.

Depending on the model (see nameplate), a 230 V, 115 V or 400 V power connection must be available at the installation site.

The distance between the wall and the rear of the appliance must be at least 15 cm. The clearance from the ceiling must not be less than 20 cm and the side clearance from walls or nearby appliances must not be less than 5 cm (Fig. 8). Sufficient air circulation in the vicinity of the appliance must be guaranteed at all times.

For appliances with castors, these need to be positioned in forward direction at all times.

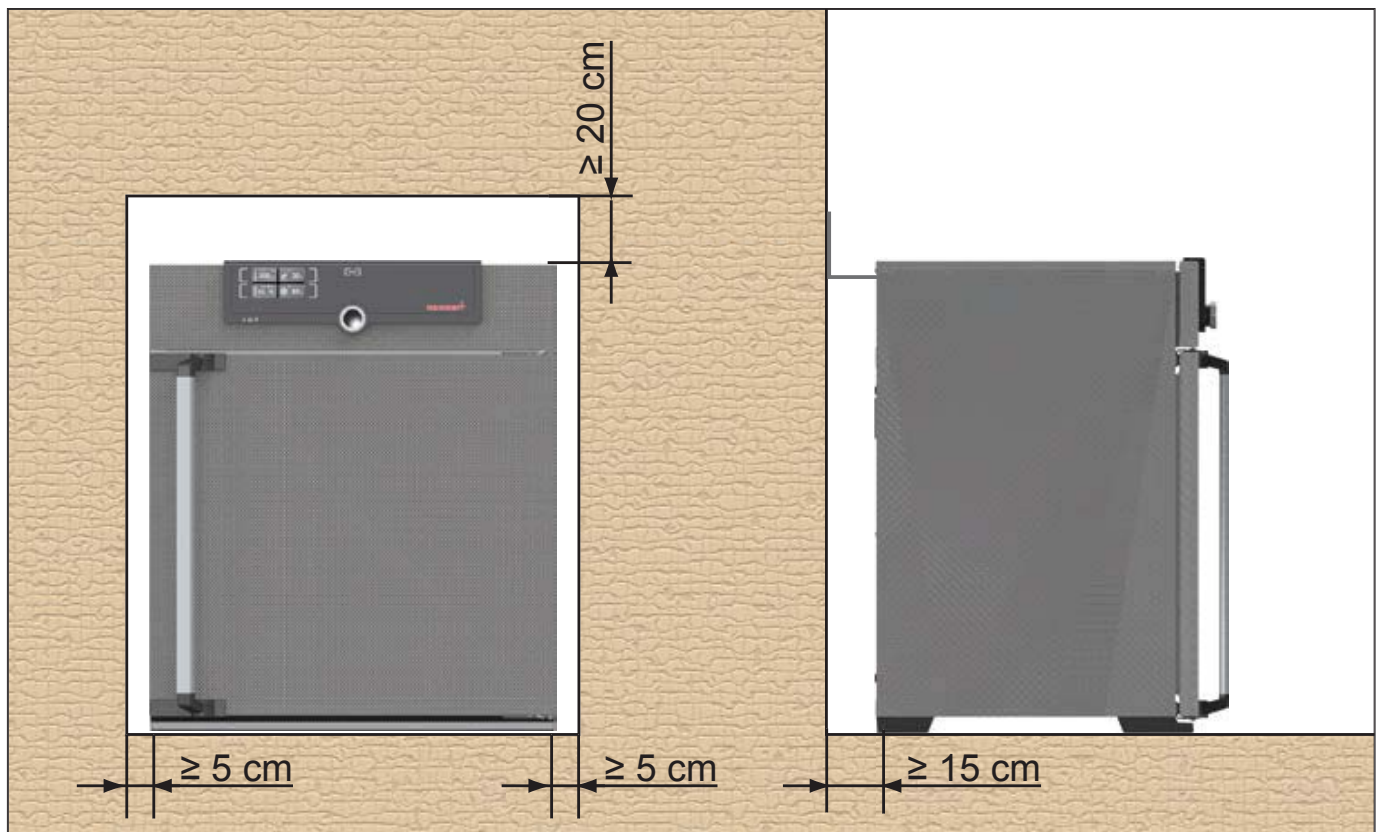









Fig. 8 Minimum clearance from walls and ceiling



### 3.6.2 Installation options

Setting up	Comments	Suitable for appliance size ...							
		30	55	75	110	160	260	450	750
<b>Floor</b> 		✓	✓	✓	✓	✓	✓	✓	✓
<b>Table</b> 	Check the load capacity first	✓	✓	✓	✓	×	×	×	×
<b>Stacked</b> 	two appliances maximum; mounting material (feet) provided	✓	✓	✓	✓	×	×	×	×
<b>Wall mounting</b> 	Separately packaged fastening material is included in the scope of delivery. Observe the assembly instructions provided.	✓	✓	✓	✓	✓	×	×	×
<b>Base</b> 	with/without castors	✓	✓	✓	✓	✓	✓	✓	×
<b>Castor frame</b> 		✓	✓	✓	✓	✓	✓	×	×
<b>Height adjustable feet</b> 		✓	✓	✓	✓	✓	✓	✓	✓

### 3.6.3 Tilt protection

Attach the appliance to a wall with the tilt protection. The tilt protection is included in the delivery.

1. As illustrated, fasten the tilt protection to the rear side of the appliance.
2. Bend the tilt protection upwards by 90 ° in the desired distance to the wall (consider the minimum distance to the wall, see Fig. 8).
3. Drill a hole, insert a plug and screw the tilt protection to a suitable wall.

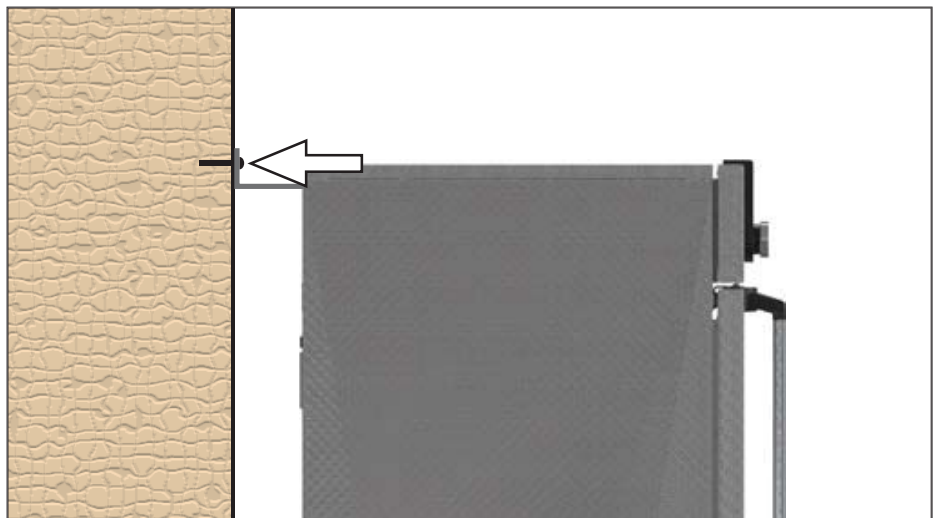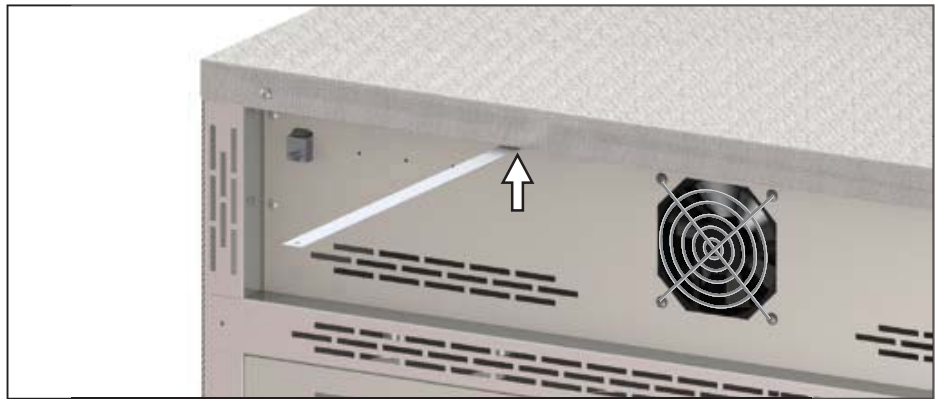

### 3.6.4 Adjusting the doors (only for model sizes 450 and 750)

For model sizes 450 and 750, it is possible to adjust doors that warp due to the floor conditions. In order to do so, every door has two adjuster screws at the top and at the bottom (Fig. 9).

**i** First, adjust the door at the top and then, if further adjustment is necessary, at the bottom as well.

1. Open the door.
2. Undo the screws.
3. Adjust the door.
4. Tighten the screws again.
5. Check door alignment.
6. If necessary, readjust.

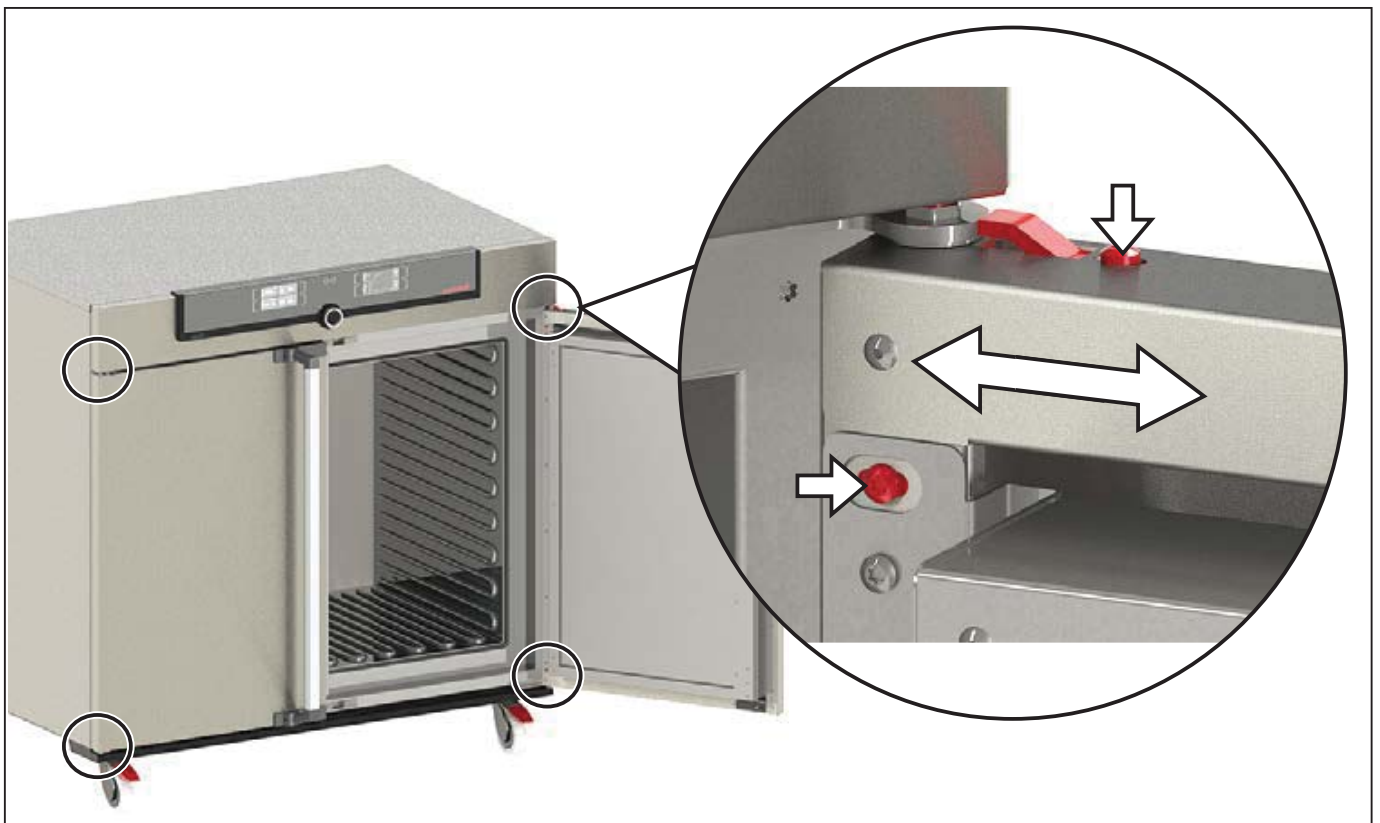


Fig. 9 Door adjustment screws



## 4. Putting into operation

### **Caution:**

The first time the appliance is operated, it must not be left unattended until it has reached the steady state.

### 4.1 Connecting the appliance

#### **Caution:**

Observe the country-specific regulations when making connections (e.g. in Germany DIN VDE 0100 with residual current circuit breaker). Observe the connection and power ratings (see nameplate and Technical data on page 13). Make sure to establish a safe PE conductor connection.

Lay the power cable so that

- ▶ it is always accessible and within reach so it can be disconnected quickly in the event of failure or emergencies;
- ▶ no one can trip over it;
- ▶ it does not come into contact with any hot parts.

#### 230/115-V appliances:

Plug the provided power cable into the rear of the appliance and connect it to a CEE 7/4 socket (Fig. 10).

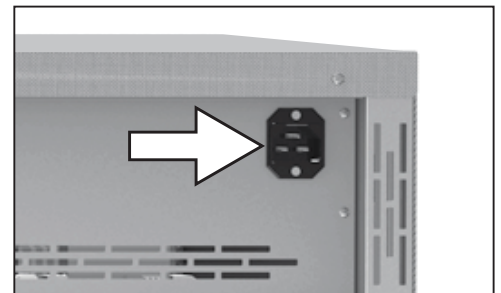


Fig. 10 Power connection  
230/115 V

#### 400V appliances:


The power cable is permanently installed. Connect the plug to a 400 V CEE coupling (Fig. 11).



Fig. 11 400 V CEE connection

### 4.2 Switching on

Switch on the appliance by pressing the On/Off switch on the front of the appliance (Fig. 12).

The starting process is shown by three animated white dots . If the dots have another colour, an error has occurred (see page 32).

**i** After the first start-up, the appliance display is set to English by default. You can change the language as described from page 35. However, to get a basic overview of operating the appliance, you should read the following chapter first.

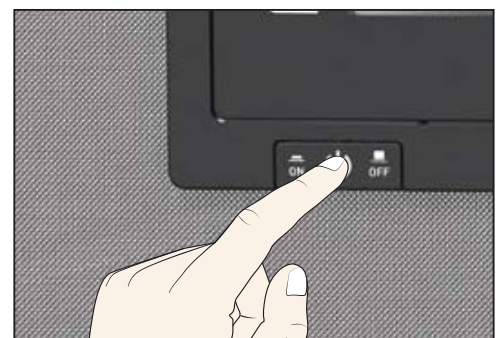


Fig. 12 Switch on appliance



## 5. Operation and control

### 5.1 Operating personnel

The appliance may only be operated by persons who are of legal age and have been instructed accordingly. Personnel who are to be trained, instructed or who are undergoing general training may only work with the appliance under the continuous supervision of an experienced person.

### 5.2 Opening the door

- ▶ To open the door, pull the door handle to the side (to the left or to the right, depending on the door variation, see Fig. 13, A) and open the door completely.
- ▶ To close the appliance, push the door closed and the door handle to the side (B).

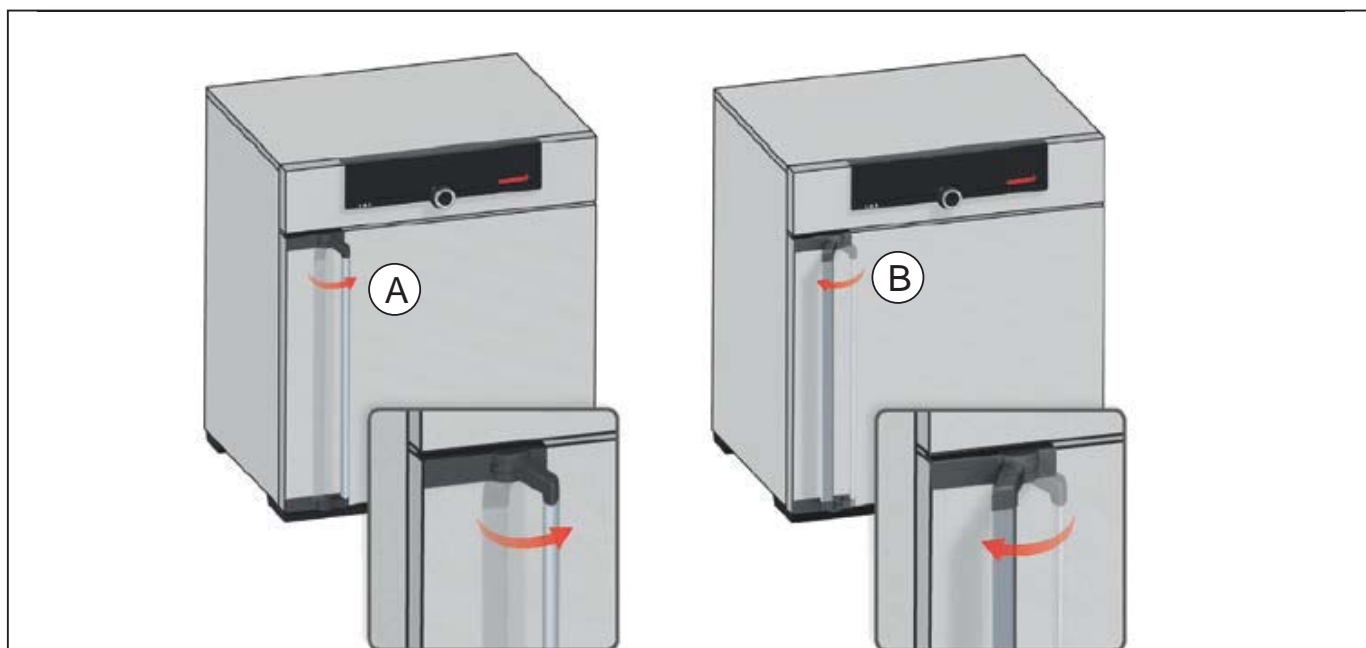


Fig. 13 Opening and closing the door



#### **Warning!**

If the door is open while the appliance is in operation, the appliance may overheat and pose a fire hazard. Do not leave the door open during operation.



#### **Warning!**

In case of appliances of a certain size, you can get accidentally locked in, which is life-threatening. Do not climb into the appliance!

## 5.3 Loading the appliance



### Warning!

When loading the appliance with an unsuitable load, poisonous or explosive vapours or gases may be produced. This could cause the appliance to explode, and persons could be severely injured or poisoned. The appliance may only be loaded with materials which do not form any toxic or explosive vapours when heated up and cannot ignite (see also Intended use on page 8). If there is any doubt as to the composition of materials, they must not be loaded into the appliance.



### i Caution:

Check the chamber load for chemical compatibility with the materials of the appliance (see page 11).

Insert the sliding steel grids or sliding shelves. The maximum number of grids / shelves and the load capacity are specified in the technical data overview on page 13.

The chamber must not be loaded too tightly, so that proper air circulation in the working chamber is guaranteed. Do not place any chamber load on the floor, touching the side walls or right below the ceiling of the working chamber (Fig. 14, see also the "correct loading" sticker on the appliance).

In case of improper loading (chamber loaded too tightly), the set temperature may be exceeded or it may take longer until it is reached.

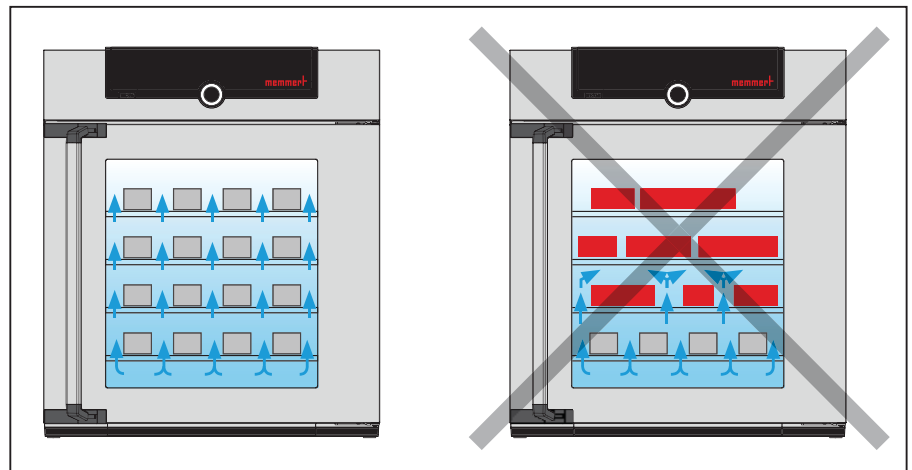


Fig. 14 Correct placement of the chamber load

i To achieve the correct heating capacity, the type of slide-in unit used – Grid or Shelf – must be set in the menu under **SETUP** (see page 39).

## 5.4 Operating the appliance

### 5.4.1 ControlCOCKPIT

In manual operation, the desired parameters are entered at the ControlCOCKPIT on the front of the appliance (Fig. 15 and Fig. 16). You can also make basic settings here (menu). Additionally, warning messages are displayed, e.g. if the temperature is exceeded.

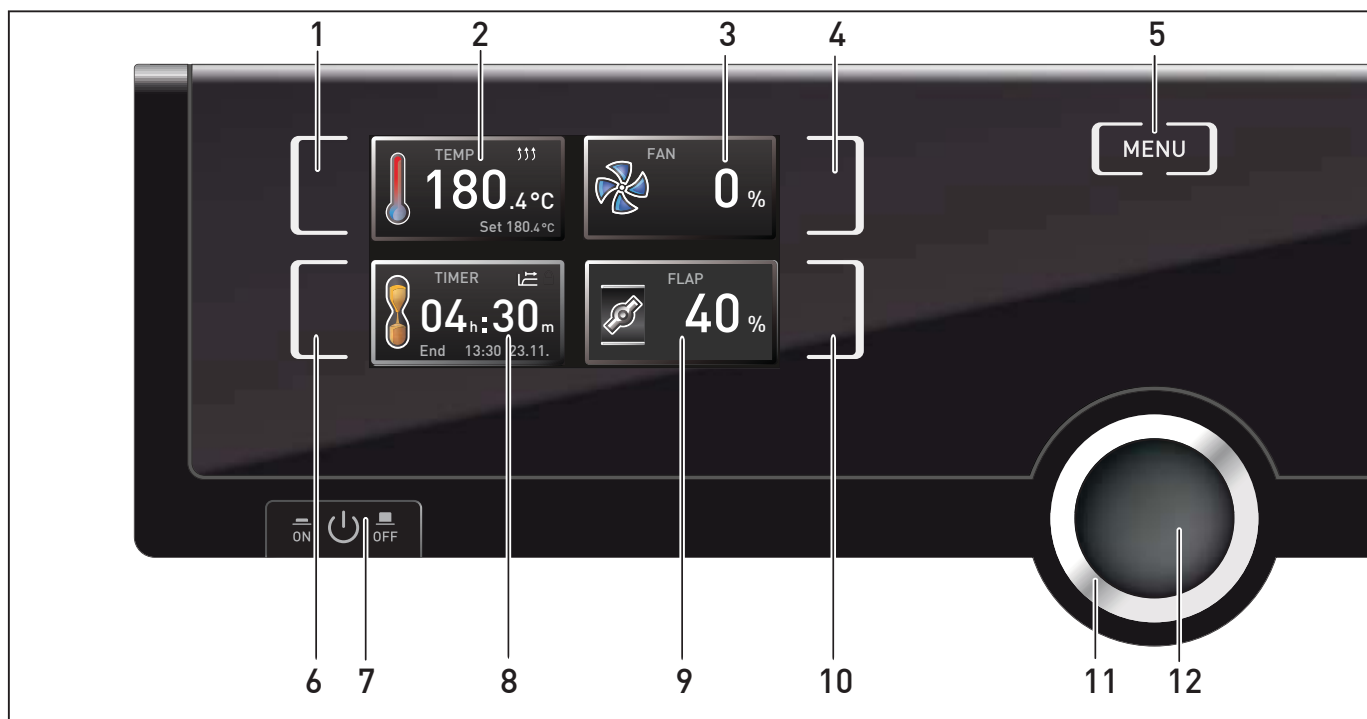


Fig. 15 ControlCOCKPIT for UFxx/IFxx appliances in operating mode

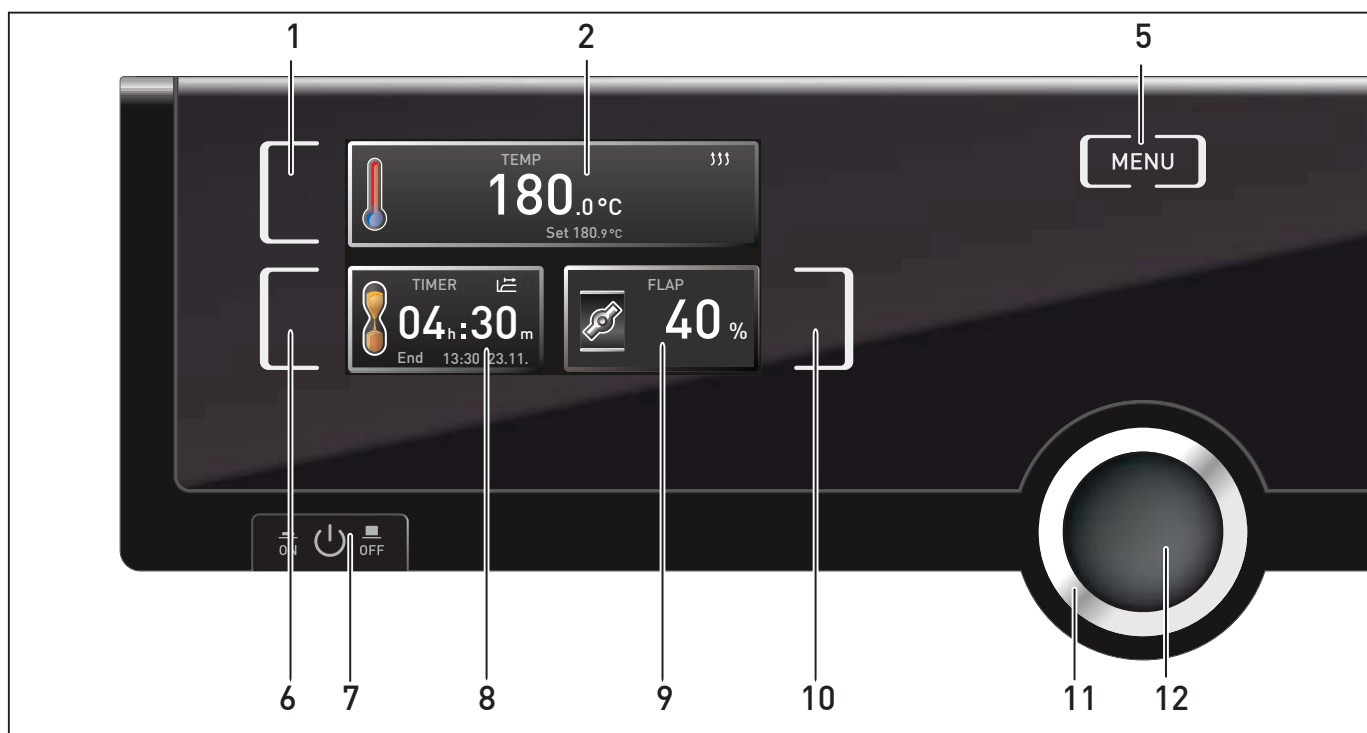



Fig. 16 ControlCOCKPIT for UNxx/INxx appliances in operating mode

- |  |   |
|--|---|
| 1 Activation key for temperature setpoint adjustment   | 8 Display digital backwards counter with target time setting, adjustable from 1 minute to 99 days |
| 2 Setpoint and actual temperature display  | 9 Air flap position display   |
| 3 Fan speed display  | 10 Activation key for air flap position adjustment  |
| 4 Activation key for fan speed setting   | 11 Turn control for setpoint adjustment   |
| 5 Switch to menu mode (see page 34)  | 12 Confirmation key (accepts setting made with the turn control)                                  |
| 6 Activation key digital backwards counter with target time setting, adjustable from 1 minute to 99 days |   |
| 7 On/Off switch  |   |



### 5.4.2 Basic operation

In general, all settings are made according to the following pattern:



1. Activate the desired parameter (e.g. temperature). To do so, press the corresponding activation key on the left or right of the respective display. The activated display is lined in colour, the other displays are dimmed. The set value is highlighted in colour.

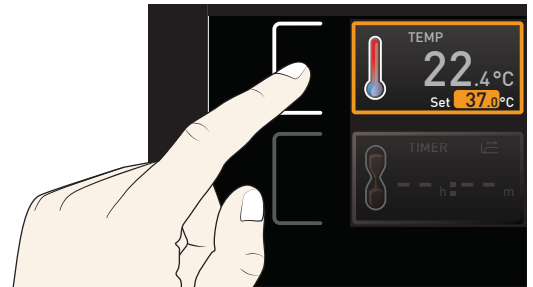

2. By turning the turn control to the left or right, adjust the set value (e.g. to 180.0 °C).

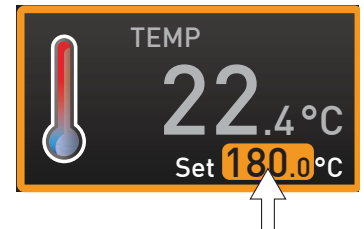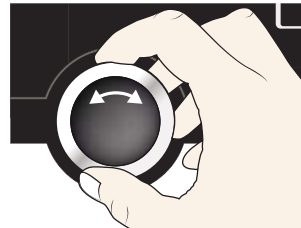


3. Save the set value by pressing the confirmation key. The display returns to normal and the appliance begins adjusting to the defined set value.

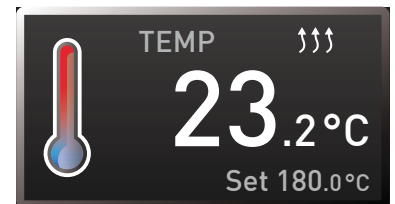

Additional parameters (air flap position etc.) can be set accordingly.

- i** If no new values are entered or confirmed for approx. 30 seconds, the appliance automatically returns to the main menu and restores the former values.

If you want to cancel the setting procedure, press the activation key on the left or right of the display that you want to exit. The appliance restores the former values. Only the settings that you have confirmed by pressing the confirmation key before cancelling the setting procedure are accepted.

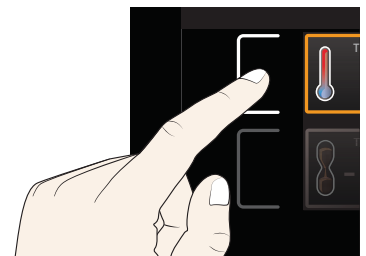

### 5.4.3 Operating modes

The appliance can be operated in different modes:

- ▶ **Manual mode:** The appliance runs in permanent operation at the values set on the ControlCOCKPIT. Operation in this mode is described in chapter 5.4.4.
- ▶ **Operation with digital backwards counter with target time setting, adjustable from 1 minute to 99 days (Timer):** The appliance runs at the values set until the timer has elapsed. Operation in this mode is described in chapter 5.4.5.
- ▶ **via remote control** (see page 39)

### 5.4.4 Manual mode

In this operating mode, the appliance runs in permanent operation at the values set on the ControlCOCKPIT.

#### Adjustment options


As described in chapter 5.4.2, you can set the following parameters after pressing the corresponding activation key (in any sequence):

#### Temperature

Adjustment range: model dependent (see nameplate and technical data on page 13)


**i** Heating operation is indicated by the ↑↑↑ symbol.

**i** You can select °C or °F as the temperature unit displayed (see page 37).

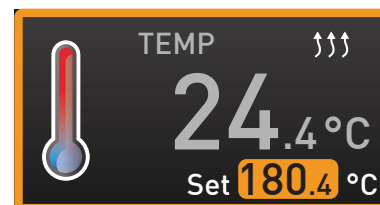

#### Air flap position

Adjustment range: 0 % (closed, recirculating operation) to 100 % (completely opened, fresh air operation) in steps of 10%

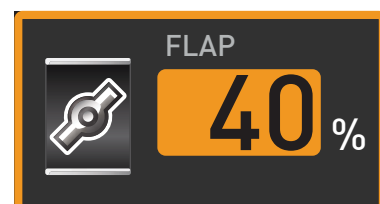

#### Fan speed

(only for UFxx/IFxx appliances)


Adjustment range: 0 to 100 % in steps of 10%





### 5.4.5 Operation with digital backwards counter with target time setting, adjustable from 1 minute to 99 days (Timer)

In timer operation, you can adjust the time the appliance runs at the set value.

1. Press the activation key to the left of the timer display. The timer display is activated.

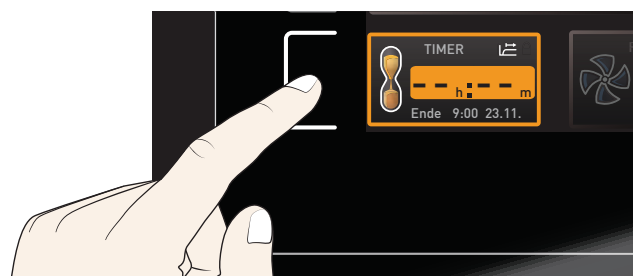


2. Turn the turn control until the desired duration is displayed – in this example 4 hours 30 minutes. The approximate end time is shown beneath, in a smaller font.

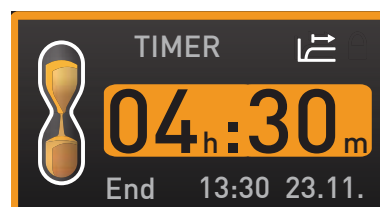


**i** Up to a duration of 23 hours 59 minutes, the time is displayed in hh:mm (hours:minutes) format. For 24 hours and more, the format dd:hh (days:hours) is used. The maximum duration adjustable is 99 days 00 hours.


- Press the confirmation key.




The display now shows the remaining time in a large font and the approximate end time in a smaller font beneath.

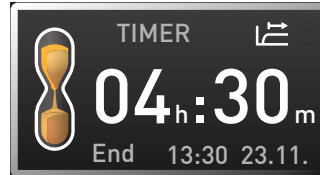


- Now, as described under 5.4.2, set the individual values for temperature, air flap position etc. which you want the appliance to operate at. The set values can be changed at any time while the timer elapses. The changes are effective immediately.

**i** In Setup, you can choose if the timer should run setpoint-dependent or not. This determines whether the timer should not start until a tolerance band around the set temperature is reached or whether it should start right after activation (see page 39). If the timer runs setpoint-dependent, this is indicated by the  symbol in the timer display.

When the timer has elapsed, the display shows 00h:00m. All functions (heating etc.) are switched off. If a fan had been active, it will keep on running for a short safety period. In addition, an acoustic alarm sounds, which can be turned off by pressing the confirmation key.

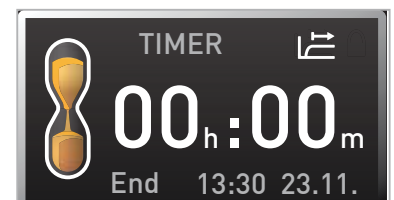

To deactivate the timer, open the timer display by pressing the activation key again and then turning the turn control to reduce the timer setting until --:-- is displayed. Confirm with the confirmation key.

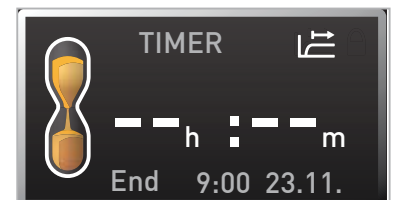

## 5.5 Temperature monitoring

The appliance is equipped with a double overtemperature protection (mechanical/electronic) in accordance with DIN 12 880. This serves to avoid damage to the chamber load and/or appliance in case of a malfunction:

- ▶ Electronic temperature monitoring (TWW/TWB) (TWB only if equipped with a second temperature sensor, option A6)
- ▶ mechanical temperature limiter (TB)

### 5.5.1 Electronic temperature monitoring

The monitoring temperature of the electronic temperature monitoring is measured via the Pt100 temperature sensor in the interior of the chamber. The type of temperature monitoring (TWW/TWB) and the monitoring temperature are set in menu mode in the Setup display (see page 38). The setting made applies to all operating modes.

If the manually set monitoring temperature is exceeded, temperature monitoring takes over temperature control and begins to regulate the monitoring temperature (TWW, Fig. 17) or switches off the heating (TWB, Fig. 18).

**i** The two types of temperature monitoring are only available for appliances equipped with a second temperature sensor (option A6). For appliances with only one temperature sensor, only TWW is available.

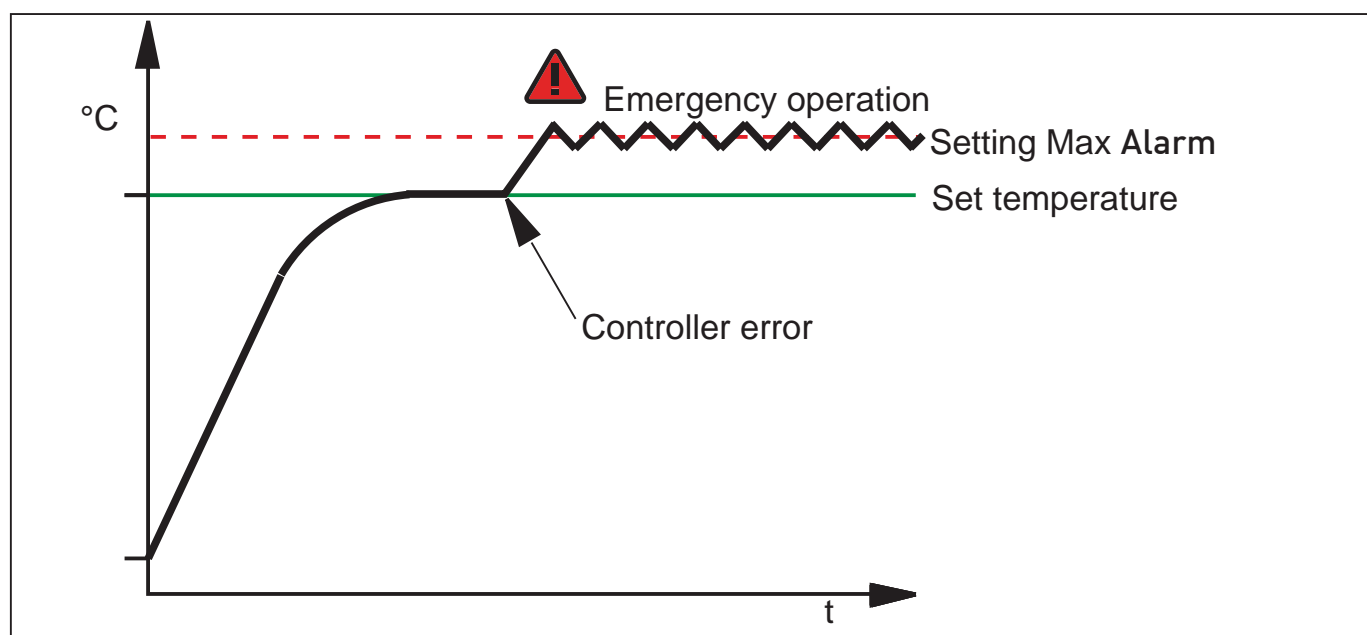


Fig. 17 Schematic diagram of how the TWW temperature monitoring system works

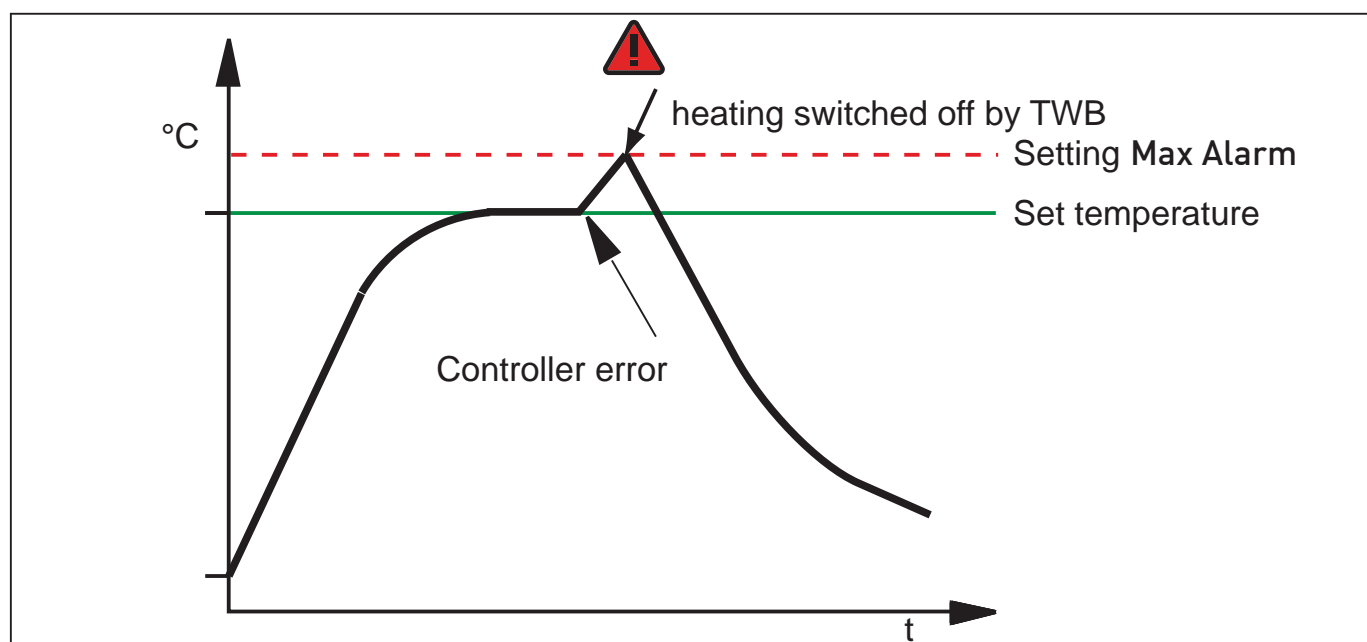


Fig. 18 Schematic diagram of how the TWB temperature monitoring works (only if equipped with a second temperature sensor, option A6)




### 5.5.2 Mechanical temperature monitoring: Temperature limiter (TB)

The appliance is equipped with a mechanical temperature limiter (TB) of protection class 1 in accordance with DIN 12 880.

If the electronic monitoring unit should fail during operation and the factory-set maximum temperature is exceeded by approx. 20 °C, the temperature limiter, as the final protective measure, switches off the heating permanently.

### 5.5.3 Function

If temperature monitoring has been triggered, this is indicated by the temperature display: the actual temperature is highlighted in red and a warning symbol  is shown (Fig. 19). The type of temperature monitoring triggered is shown beneath the temperature: TB for mechanical and TWW or TWB for electronic temperature monitoring. The alarm is additionally signalled by an intermittent acoustic signal, which can be turned off by pressing the confirmation key. Information on what to do in this case are provided in the chapter Malfunctions, warning and error messages from page 31.

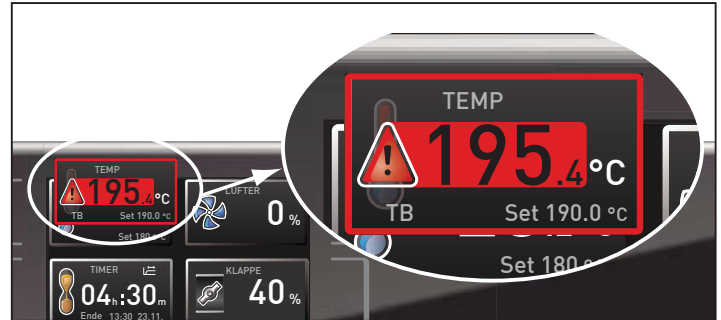


Fig. 19  
Temperature monitoring triggered

## 5.6 Ending operation



### Warning!

Depending on the operation performed, the surfaces in the working chamber and the chamber load may still be very hot after the appliance is switched off. Touching these surfaces can cause burns. Wear heat-resistant protective gloves or wait until the appliance cools down.

1. Switch off active appliance functions (turn back the set values).
2. Remove the chamber load.
3. Switch off the appliance (Fig. 20).

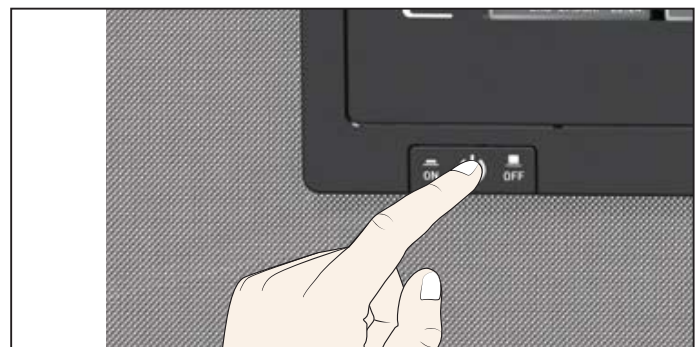


Fig. 20 Switch off appliance

## 6. Malfunctions, warning and error messages






### Warning!

After removing covers, live parts may be exposed. You may receive an electric shock if you touch these parts. Malfunctions requiring work inside the appliance may only be rectified by electricians. Observe the separate service manual for this.


Do not try to rectify appliance errors yourself but contact the MEMMERT customer service department (see page 2) or an authorised service point.

In case of enquiries, please always specify the model and appliance number from the nameplate (see page 12).

### 6.1 Warning messages of the temperature monitoring function

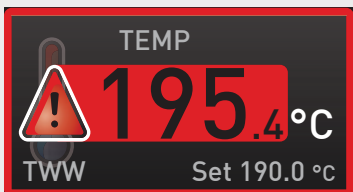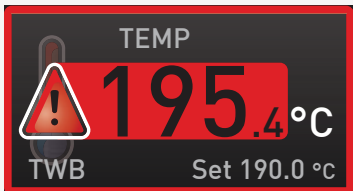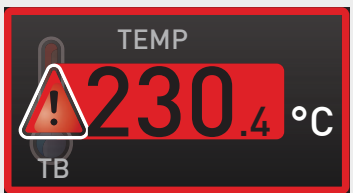Description	Cause	Action	See
Temperature alarm and "TWW" are displayed 	The adjustable undertemperature / overtemperature controller (TWW) has assumed heating control.	Increase the difference between the monitoring and setpoint temperature – by either increasing the max value of the temperature monitoring ( <b>MAX temp</b> ) or decreasing the setpoint temperature. If the alarm continues: Contact customer service	page 38  page 2
Temperature alarm and "TWB" are displayed 	The electronic temperature limiter (TWB) permanently switched off heating.	Deactivate the alarm by pressing the confirmation key. Increase the difference between the monitoring and setpoint temperature – by either increasing the max value of the temperature monitoring ( <b>MAX temp</b> ) or decreasing the setpoint temperature. If the alarm continues: Contact customer service	page 38  page 2
Temperature alarm and TB are displayed 	The mechanical temperature limiter (TB) permanently switched off heating.	Switch off the appliance and leave to cool down. Contact customer service and have the error rectified (e.g. by replacing the temperature sensor).	page 2

## 6.2 Malfunctions, operating problems and appliance errors

Error description	Cause of errors	Rectifying errors	See
Displays are dark	External power supply was interrupted	Check the power supply	page 22
	Miniature fuse, appliance fuse or power module faulty	Contact customer service	page 2
Individual or all displays cannot be activated	The appliance is in timer or remote control mode (mode "Write" or "Write + Alarm")	Wait until the end of the timer or switch off the remote control	
Displays suddenly look different	Appliance is in "wrong" mode	Change to operating or menu mode by pressing the <b>MENU</b> key	
Error message E-3 in the temperature display 	Temperature sensor defective.	<ul style="list-style-type: none"> <li>▶ Switch off appliance.</li> <li>▶ Remove the chamber load</li> <li>▶ Contact customer service</li> </ul>	page 2
When switching on the appliance, the start animation is displayed in another colour than white ●●●	▶ Cyan ●●●: Not enough storage space on the SD card	Contact customer service	page 2
	▶ Red ●●●: The system files could not be loaded	Contact customer service	page 2
	▶ Orange ●●●: The fonts and images could not be loaded	Download the firmware update at <a href="http://memmert.com">memmert.com</a> and install it	

## 6.3 Power failure



### Warning!

Depending on the operation performed, the surfaces in the interior and the chamber load may still be very hot after power loss. Additionally, depending on the duration of the power loss, the appliance might heat up again after power supply has been restored (see below). Touching these surfaces can cause burns. Wear heat-resistant protective gloves or wait until the appliance cools down first.

In case of a power failure, the appliance operates as follows:

#### In manual mode

After power supply has been restored, operation is continued with the parameters set. The time and the duration of the power failure is documented in the protocol log memory.

#### In timer mode

In case of an interruption of the power supply of less than 60 minutes, the current timer is continued from the point at which it was interrupted. For interruptions of the power supply longer than this, all appliance functions (heating, fan etc.) are switched off and the air flap is opened.

#### In remote control mode:

The previous values are restored.

## 7. Menu mode


In menu mode, you can make basic settings as well as adjust appliance parameters.

### **i Caution:**

Before changing menu settings, read the description of the respective functions on the following pages to avoid possible damage to the appliance and/or chamber load.

To enter menu mode, press the MENU key.

**i** To exit the menu mode at any time, press the MENU key again. The appliance then returns to manual mode. Only changes accepted by pressing the confirmation key are saved.

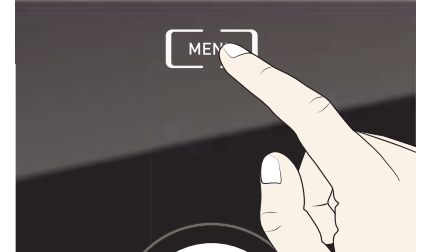

### 7.1 Overview

Press the MENU key to change between the displays in menu mode:

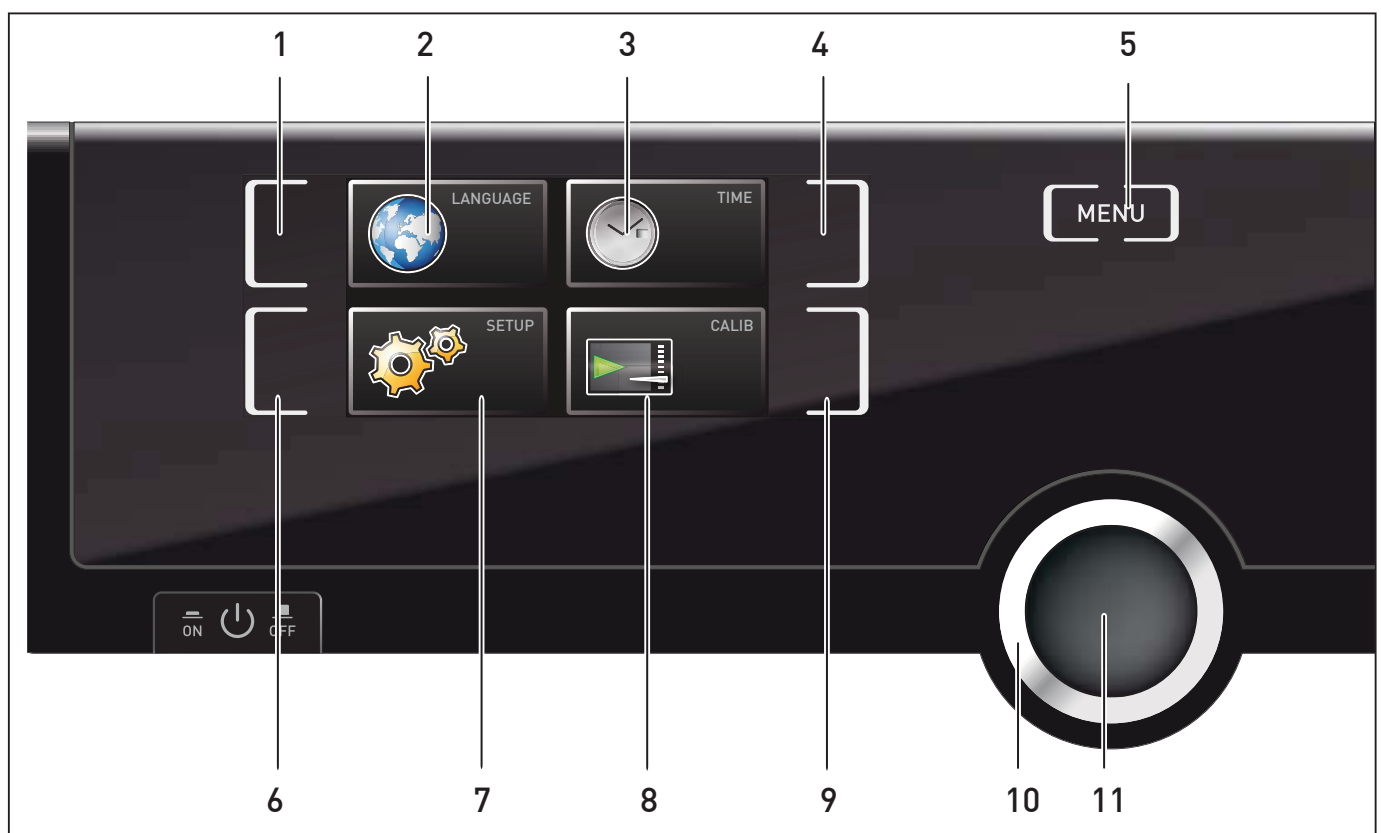



Fig. 21 ControlCOCKPIT in menu mode

- |   |  |
|---|--|
| 1 Language selection activation key               | 7 Setup display (basic appliance settings)                       |
| 2 Language selection display                      | 8 Adjustment display   |
| 3 Date and time display                           | 9 Adjustment activation key                                      |
| 4 Date and time setting activation key            | 10 Turn control for adjustment                                   |
| 5 Return to manual mode                           | 11 Confirmation key (accepts setting made with the turn control) |
| 6 Setup activation key (basic appliance settings) |  |


## 7.2 Basic operation in menu mode using the example of language selection

In general, all settings in menu mode are done just like in manual mode: Activate the respective display, use the turn control for setting and press the confirmation key to accept the change. A more detailed description is provided in the following, using the example of language selection.



1. Activate the desired parameter (in this example the language). To do so, press the corresponding activation key on the left or right of the respective display. The activated display is enlarged.

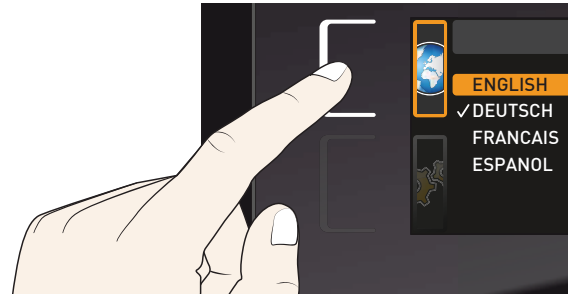



- i** If you want to exit or cancel your settings, again press the activation key which you have used to activate the display. The appliance returns to the menu overview. Only the settings that you have confirmed by pressing the confirmation key before cancelling the setting procedure are accepted.

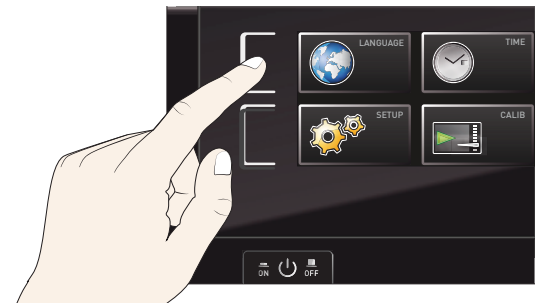


2. With the turn control, select the desired new setting, e.g. Español (Spanish).

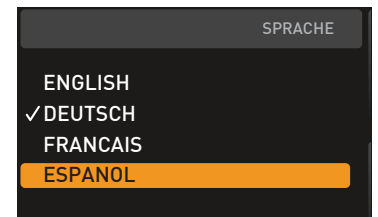

3. Save the setting by pressing the confirmation key.

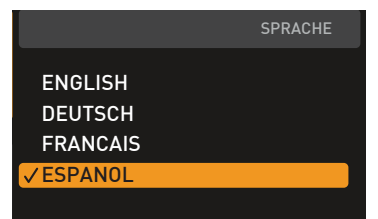



4. To return to the menu overview, press the activation key again.

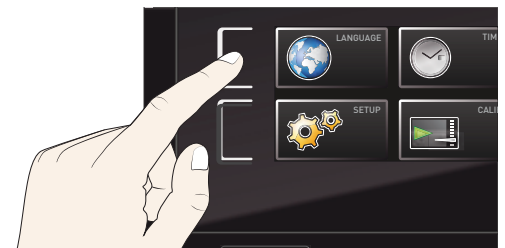

You can now

- ▶ activate another menu function by pressing the corresponding activation key or
- ▶ return to manual mode by pressing the MENU key.

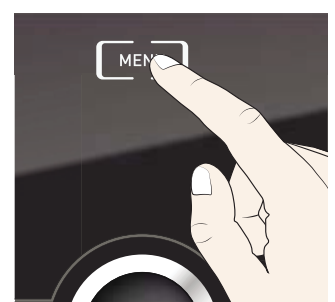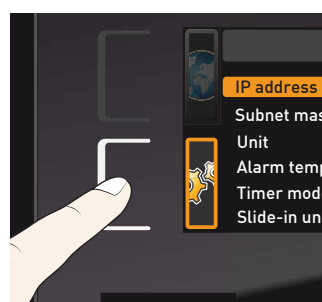

All other settings can be made accordingly. The settings possible are described in the following sections.

**i** If no new values are entered or confirmed for approx. 30 seconds, the appliance automatically returns to the main menu and restores the former values.


## 7.3 Setup

In the **SETUP** display, you can set the following parameters:

- ▶ the **IP address** and **Subnet mask** of the appliance's Ethernet interface (for connection to a network)
- ▶ the **Unit** of the temperature display (°C or °F, see page 37)
- ▶ the type of temperature monitoring (TWW or TWB, **Alarm Temp**, only if equipped with a second temperature sensor, option A6) and the trigger temperature of the monitoring function (**Max alarm**, see page 38)
- ▶ how the digital backwards counter with target time setting works (**Timer mode**, see page 39)
- ▶ the type of the slide-in unit (Grid or Shelf, see page 39)
- ▶ Remote control (see page 39)
- ▶ Gateway (see page 40)

**i** If the **SETUP** menu contains more entries than can be displayed, this is indicated by the display "1/2". This means that there is a second „page“ of entries.

To display the hidden entries, use the turn control to scroll beyond the lowest entry. The page display changes to "2/2".

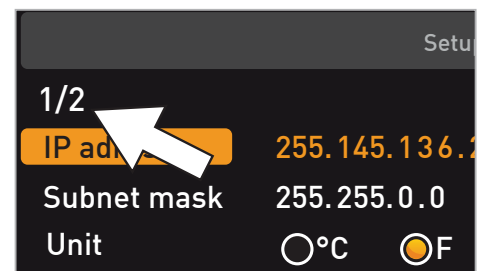

### 7.3.1 IP address and subnet mask

If you want to operate one or more appliances in a network, each appliance must have its own unique IP address for identification. By default, each appliance is delivered with the IP address 192.168.100.100.


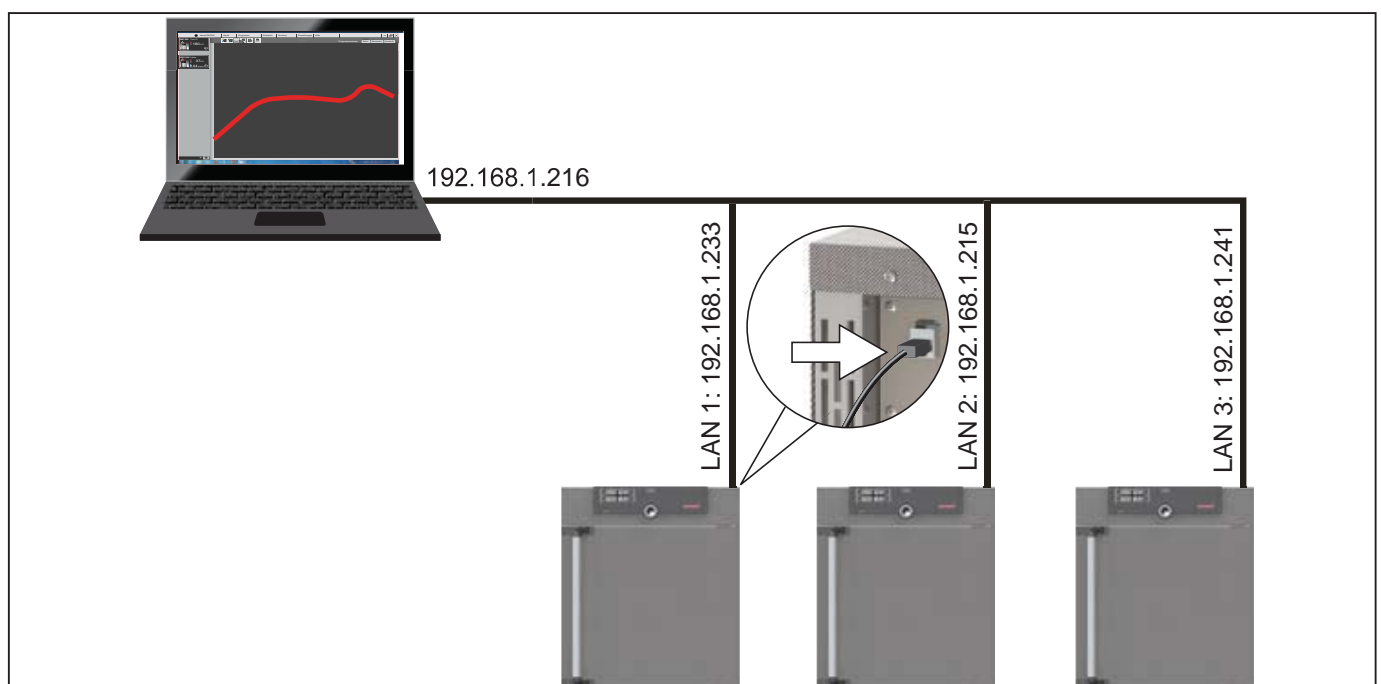




Fig. 22 Operation of several appliances in a network (schematic example)




1. Activate the **SETUP** display. The entry **IP address** is automatically highlighted.

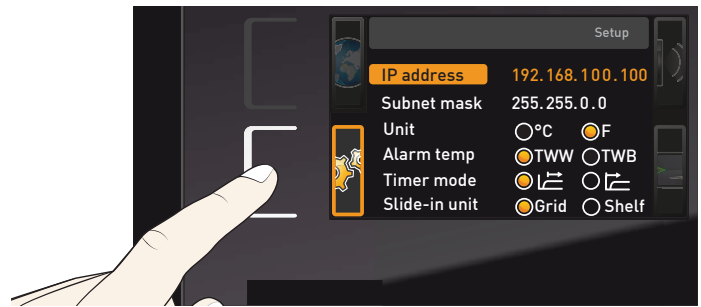



2. Accept the selection by pressing the confirmation key. The first three digits of the IP address are automatically selected.

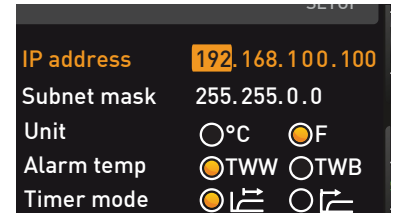



3. With the turn control, set the new number, e.g. 255.

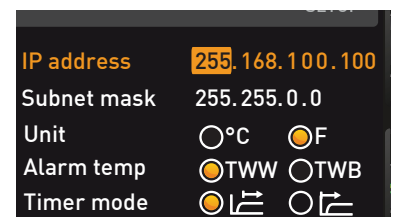

4. Accept the selection by pressing the confirmation key. The next three digits of the IP address are automatically selected. Setting these is done with the turn control according to the description above.

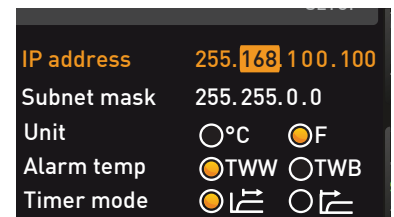

5. After setting the last three digits, accept the new IP address by pressing the confirmation key. The selection returns to the overview.

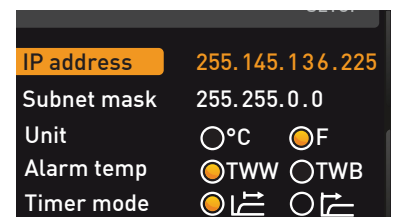

The subnet mask is set accordingly.

### 7.3.2 Unit


Here, you can choose whether the temperature is displayed in °C or °F.

### 7.3.3 Temperature monitoring (Alarm Temp and Max Alarm)
















Here, the type of monitoring function that should be activated (TWW or TWB, description from page 28) can be set (**Alarm Temp**), as well as the temperature at which the automatic temperature monitoring should be triggered (**Max alarm**).

**i** The selection option TWW/TWB is only available for appliances with a second temperature sensor (option A6).

**i** The monitoring temperature must be set sufficiently high above the maximum set temperature. We recommend 5 to 10 K difference for UNxx/UFxx and 1 to 3 K difference for INxx/IFxx.

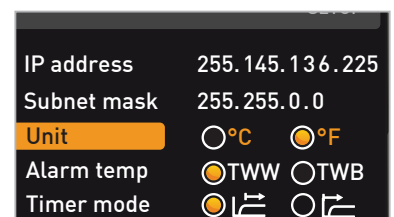

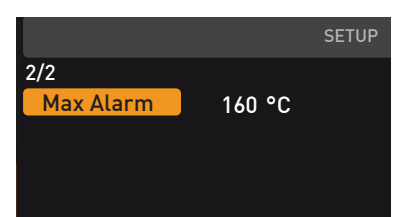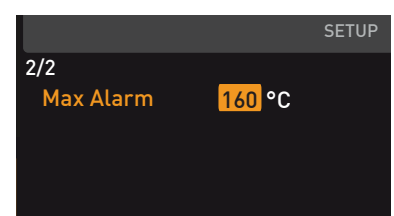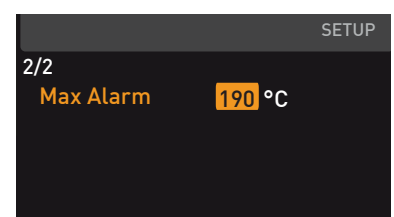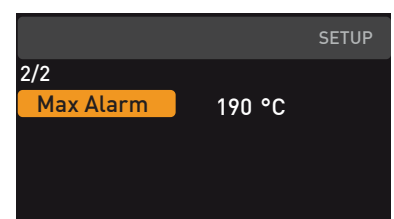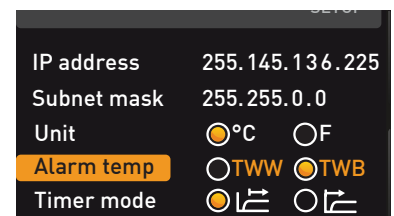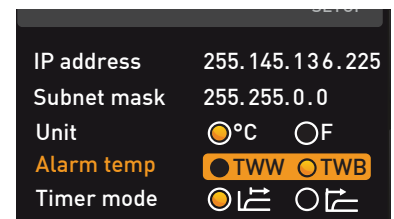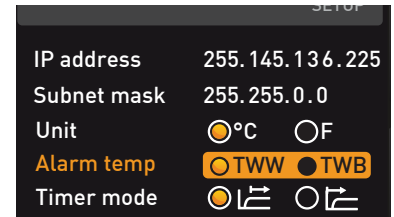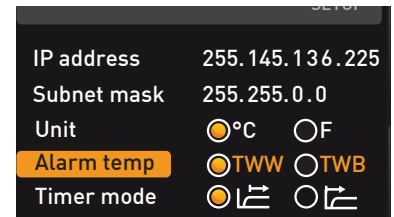

1. Activate the **SETUP** display and select **Alarm temp** with the turn control.
2. Accept the selection by pressing the confirmation key. The adjustment options are automatically highlighted.
3. With the turn control, select the desired setting – in this example **TWB**.
4. Save the setting by pressing the confirmation key.
5. Select **Max Alarm** with the turn control.
6. Accept the selection by pressing the confirmation key. The current settings are automatically highlighted.
7. With the turn control, select the desired new trigger temperature - in this example **160 °C**.
8. Save the setting by pressing the confirmation key. The electronic temperature monitoring system will now be triggered when the actual temperature reaches 160 °C.



### 7.3.4 Timer Mode

Here, you can choose whether the digital backwards counter with target time setting (see page 27, timer) should run setpoint-dependent or not – this determines whether the timer should not start until a tolerance band of  $\pm 3$  K around the set temperature is reached (Fig. 23, B) or whether it should start right after activation (A).

IP address	255.145.136.225
Subnet mask	255.255.0.0
Unit	<input checked="" type="radio"/> °C <input type="radio"/> °F
Alarm temp	<input type="radio"/> TWW <input checked="" type="radio"/> TWB
Timer mode	<input checked="" type="radio"/>  <input type="radio"/> 

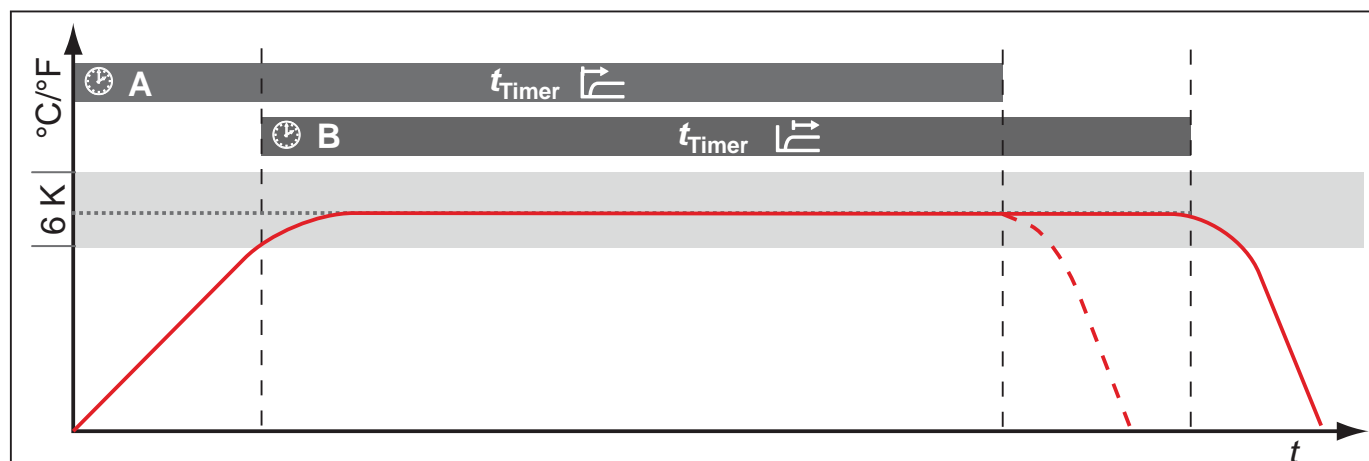


Fig. 23 Timer Mode



A Timer independent of setpoint: Timer starts right after activation

B Timer setpoint-dependent: Timer does not start until tolerance band is reached

If the temperature tolerance band is exceeded in setpoint-dependent operation, the timer will be interrupted and only be resumed when the setpoint temperature has been reached again.

### 7.3.5 Type of the slide-in unit (Grid or Shelf)


Here, you have to set the type of the slide-in unit (grid or shelf) used. The selection Shelf enables you to adjust the control function to the different air flow characteristics in the interior when using optional sliding shelves instead of the grids that are part of the standard delivery.


IP address	255.145.136.225
Subnet mask	255.255.0.0
Unit	<input checked="" type="radio"/> °C <input type="radio"/> °F
Alarm temp	<input type="radio"/> TWW <input checked="" type="radio"/> TWB
Timer mode	<input checked="" type="radio"/>  <input type="radio"/> 
Slide-in unit	<input checked="" type="radio"/> Grid <input type="radio"/> Shelf


### 7.3.6 Remote control


In the setup entry **Remote control**, you can set whether the appliance should be controlled via remote control and if so, in which mode. These settings are available:

- ▶ Off
- ▶ Read Only
- ▶ Write
- ▶ Write+Alarm

When the appliance is in remote control mode, the  symbol appears in the temperature display. In the settings **Write** and **Write+Alarm**, the appliance cannot be controlled at the ControlCOCKPIT until the remote control has been switched off (setting Off) or set to **Read Only**.

 In order to use the remote control function, programming skills and special libraries are required.


2/2	Balance	+30 %
	Remote Control	Off
	Gateway	192.168.5.1

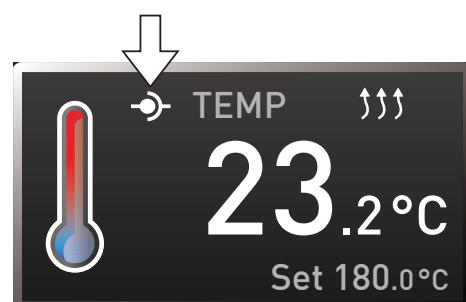

### 7.3.7 Gateway

The setup entry **Gateway** is used to connect two networks with different protocols.

The gateway is set the same way as the IP address (see page 36).

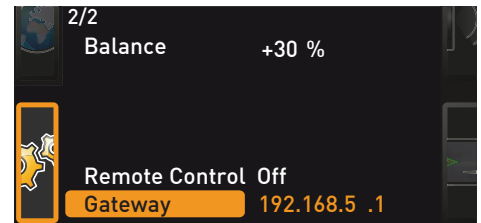


## 7.4 Date and Time


In the **Time** display, you can set date and time, time zone and daylight saving time.

**i** Always set the time zone (and summer time yes/no) before you set the date and time. Avoid changing the set time after that since this can lead to gaps or overlapping when recording measured values. If you still need to change the time, you should not run a programme immediately before or after doing so.



1. Activate the time setting. To do so, press the activation key on the right side of the **Time** display. The display is enlarged and the first adjustment option (**Date**) automatically highlighted.

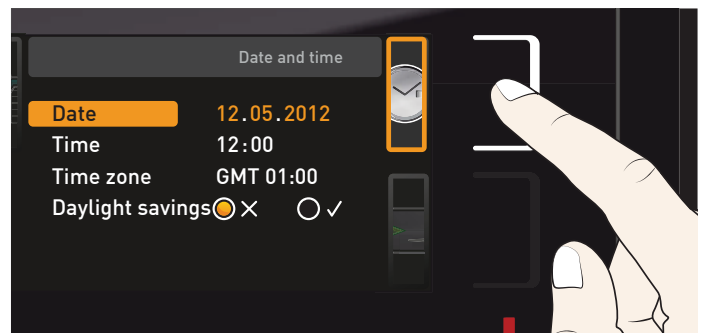



2. Turn the turn control until **Time zone** is highlighted.

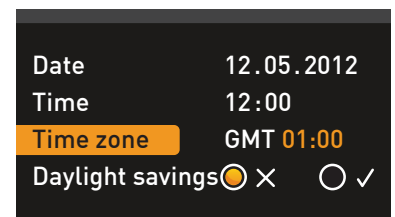



3. Accept the selection by pressing the confirmation key.

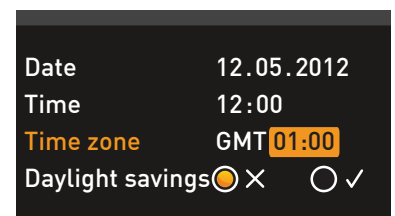


4. Set the time zone of the installation site with the turn control, e.g. 00:00 for France, Spain or Great Britain, 01:00 for Germany. Accept the selection by pressing the confirmation key.

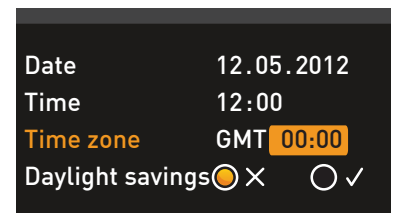

5. With the turn control, select the **Daylight savings** entry

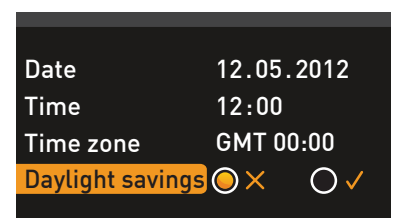


6. Accept the selection by pressing the confirmation key. The adjustment options are highlighted.



Date	12.05.2012
Time	12:00
Time zone	GMT 00:00
Daylight savings	<input type="radio"/> X <input checked="" type="radio"/> ✓


7. Set daylight savings to off (X) or on (✓) with the turn control – in this case on (✓). Save the setting by pressing the confirmation key.



Date	12.05.2012
Time	12:00
Time zone	GMT 00:00
Daylight savings	<input checked="" type="radio"/> X <input type="radio"/> ✓

**i** Daylight saving time and standard time are not changed automatically. For this reason, please keep in mind to adjust them at the beginning of each period.

8. Now, set date (day, month year) and time (hours, minutes) in the same way. Accept the selection by pressing the confirmation key.




Date	27.05.2012
Time	12:00
Time zone	GMT 00:00
Daylight savings	<input type="radio"/> X <input checked="" type="radio"/> ✓

## 7.5 Calibration

The appliances are temperature calibrated and adjusted at the factory. In case readjustment should be necessary later on – for example due to influence of the chamber load – the appliance can be calibrated customer-specifically using three calibration temperatures of your choice:

- ▶ Cal1      Temperature calibration at low temperature
- ▶ Cal2      Temperature calibration at medium temperature
- ▶ Cal3      Temperature calibration at high temperature

To guarantee perfect control, we recommend to calibrate the appliance once a year.

 For temperature adjustment, you will need a calibrated reference measuring device.


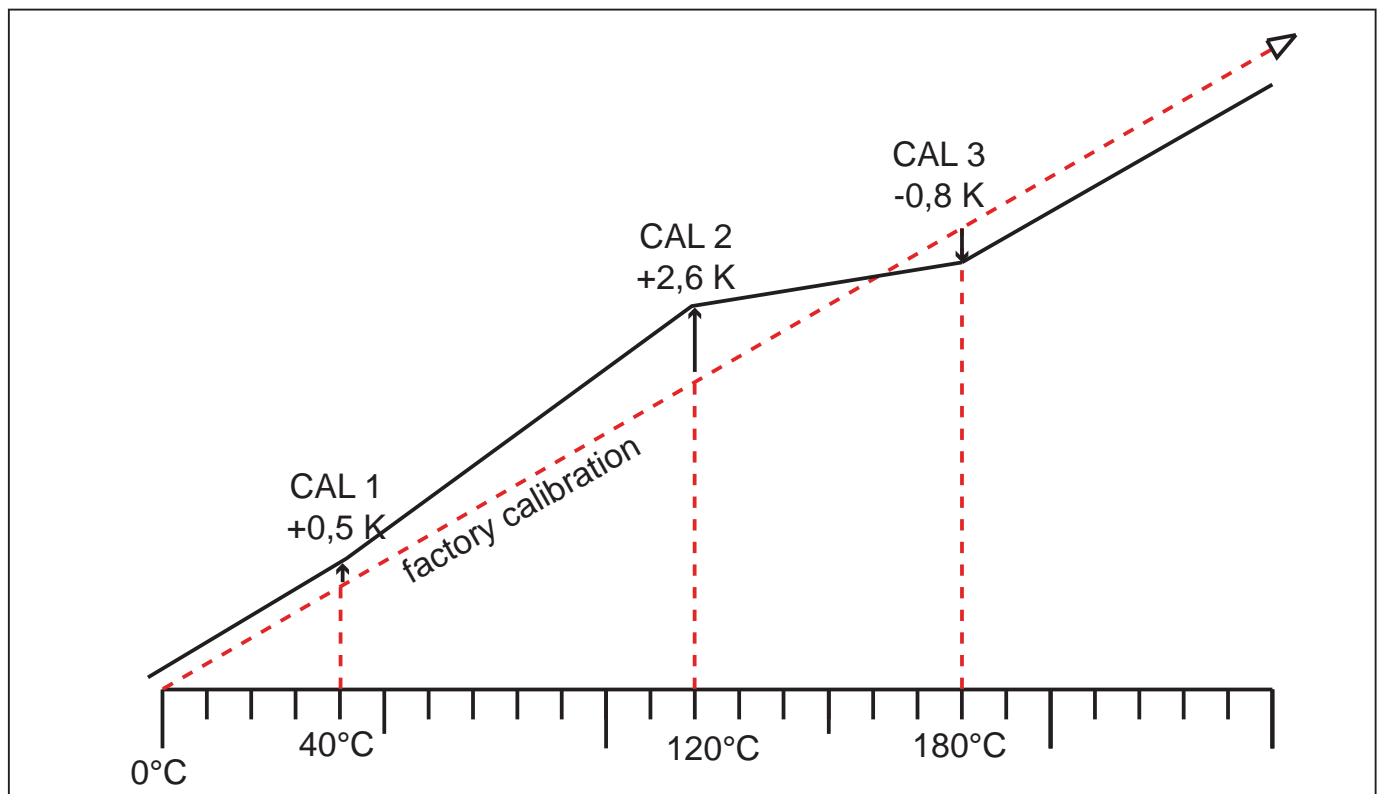



Fig. 24 Schematic example of temperature adjustment

Example: Temperature deviation at 120 °C should be corrected.

1. Activate the adjustment setting. To do so, press the activation key on the right side of the **CALIB** display. The display is enlarged and the first calibration temperature – in this case 40 °C – automatically highlighted.
2. Press the confirmation key repeatedly, until the calibration temperature Cal2 is selected.

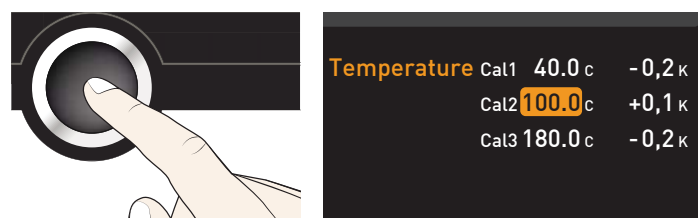


- With the turn control, set the calibration temperature Cal2 to 120 °C.



Temperature	Cal1	40.0 c	-0,2 K
	Cal2	120.0 c	+0,1 K
	Cal3	180.0 c	-0,2 K

- Save the setting by pressing the confirmation key. The corresponding calibration value is automatically highlighted.



Temperature	Cal1	40.0 c	-0,2 K
	Cal2	120.0 c	+0,1 K
	Cal3	180.0 c	-0,2 K



- Set the calibration value to 0.0 K and accept the setting by pressing the confirmation key.





Temperature	Cal1	40.0 c	-0,2 K
	Cal2	120.0 c	0,0 K
	Cal3	180.0 c	-0,2 K

- Position the sensor of a calibrated reference instrument centrally in the appliance's working chamber.

- Close the door and, in manual mode, adjust the set temperature to 120 °C.

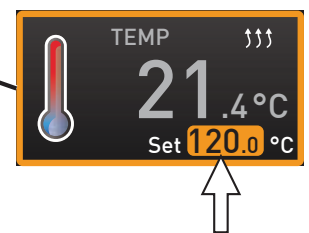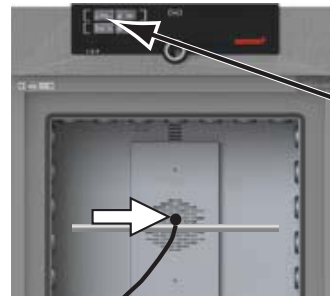

- Wait until the appliance reaches the set temperature and displays 120 °C. The reference instrument for example displays 122.6 °C.


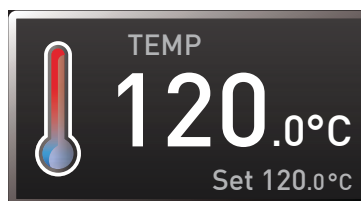


- In the SETUP, adjust the calibration value Cal2 to +2.6 K (actual value measured minus setpoint temperature) and save the setting by pressing the confirmation key.



Temperature	Cal1	40.0 c	-0,2 K
	Cal2	120.0 c	+2,6 K
	Cal3	180.0 c	-0,2 K

- After the calibration procedure, the temperature measured by the reference instrument should now also be 120 °C.

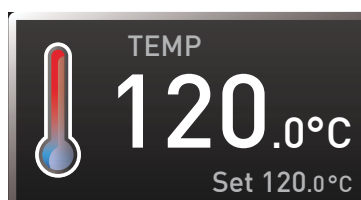

With Cal1, a calibration temperature below Cal2 can be programmed accordingly, and with Cal3, a temperature above. The minimum difference between the Cal values is 20 K for universal ovens UNxx/UFxx and 10 K for incubators INxx/IFxx.




If all calibration values are set to 0.0 K, the factory calibration settings are restored.



## 8. Maintenance and service

---

### 8.1 Cleaning

**Warning!**

**Danger due to electric shock. Before doing any maintenance work, pull out the mains plug.**

---

**Warning!**

**In case of appliances of a certain size, you can get accidentally locked in, which is life-threatening. Do not climb into the appliance!**

---

**Caution!**

**Danger of cuts due to sharp edges. Always wear gloves when working in the chamber interior.**

---

#### 8.1.1 Working chamber and metal surfaces

Regular cleaning of the easy-to-clean working chamber prevents build up of material remains that could impair the appearance and functionality of the stainless steel working chamber over time.

The metal surfaces of the appliance can be cleaned with normal stainless steel cleaning agents. Make sure that no rusty objects come into contact with the working chamber or with the stainless steel housing. Rust deposits can lead to an infection of the stainless steel. If rust spots should appear on the surface of the working chamber due to impurities, the affected area must be immediately cleaned and polished.

#### 8.1.2 Plastic parts

Do not clean the ControlCOCKPIT and other plastic parts of the appliance with caustic or solvent-based cleaning agents.

#### 8.1.3 Glass surfaces

Glass surfaces can be cleaned with a commercially available glass cleaner.


### 8.2 Regular maintenance

Once a year, grease the moving parts of the doors (hinges and lock) with thin silicone grease and check that the hinge screws are not loose.

To guarantee perfect control, we recommend to calibrate the appliance once a year (see page 42).

### 8.3 Repairs and service

---

**Warning!**

**After removing covers, live parts may be exposed. You may receive an electric shock if you touch these parts. Disconnect the mains plug before removing any covers. Any work inside the appliance may only be performed by qualified electricians.**

---



Repairs and service work are described in a separate service manual.

---

## 9. Storage and disposal

### 9.1 Storage

The appliance may only be stored under the following conditions:

- ▶ in a dry and enclosed, dust-free room
- ▶ frost-free
- ▶ disconnected from the power supply

### 9.2 Disposal

This product is subject to the Directive 2002/96/EC on Waste Electrical and Electronic Equipment (WEEE) of the European Parliament and of the Council. This appliance has been brought to market after August 13<sup>th</sup>, 2005 in countries which have already integrated this directive into their national laws. It may not be disposed of in normal household waste. For disposal, please contact your dealer or the manufacturer. Any appliances that are infected, infectious or contaminated with materials hazardous to health are excluded from return. Please also observe all other regulations applicable in this context.

Before disposing of the appliance, please render the door locking mechanism unusable, for example, to prevent playing children from being locked inside the appliance.

There is a lithium battery in the ControlCOCKPIT of the appliance. Remove it and dispose of it in accordance with the regulations in your country (Fig. 25).

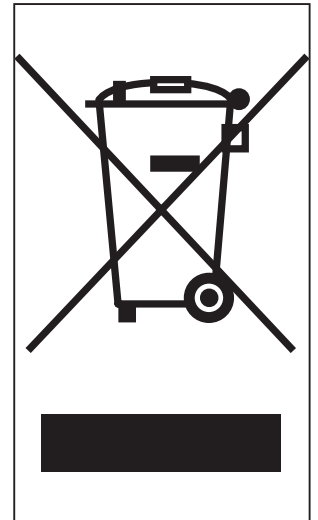


Fig. 25 Removing the lithium battery

#### Note for Germany:

The appliance may not be left at public or communal recycling or collection points.

# Index

- A**  
Accessories 15  
Activation key 26  
Adjustment 42  
Air flap position 27  
Air supply 11  
Alarm 37  
Alarm temperature 38  
Ambient conditions 14  
Ambient temperature 15  
Appliance error 32  
AtmoCONTROL 3, 12, 15
- B**  
Basic device settings 34  
Basic settings 34
- C**  
Calibration 42  
Carrying 16  
Cause of errors 32  
Chamber load 24  
Changes 8  
Cleaning 44  
Clock time 40  
Communication interfaces 12  
Compensation correction value 43  
Connections 12  
ControlCOCKPIT 25  
Convection 11  
Customer service 2
- D**  
Date and time 40  
Declaration of conformity 14  
Decommissioning 45  
Delivery 16, 17, 22  
Digital backwards counter 27  
Dimensions 14  
Disposal 45  
Door 23
- E**  
Electrical connection 12  
Electrical connections 22  
Electronic temperature monitoring 29  
Emergency 9  
Ending operation 30  
Error description 32  
Error messages 31  
Explosion protection 8
- F**  
factory calibration 43  
Fan speed 27  
Fehlermeldung 32  
Forklift truck 17  
Function 11
- G**  
Gateway 40  
Graph 30  
Grid 39
- H**  
Hazards 7
- I**  
Installation site 18  
Intended use 8  
Interfaces 12  
IP address 36
- L**  
Language selection 35  
Loading the appliance 24  
Log memory 33
- M**  
Maintenance 44  
Malfunctions 9, 31  
Manufacturer 2  
Material 11  
Mechanical temperature monitoring 30  
Menu 34, 40  
Minimum clearances 18
- N**  
Nameplate 12  
Network 12, 36  
Normal mode 26, 27
- O**  
Operating 23  
Operating modes 26  
Operating personnel 7, 23  
Operating problems 32  
Operation 23
- P**  
Packaging material 17  
Power failure 33  
Product safety 7  
Putting into operation 22
- R**  
Rectifying errors 32  
Regular maintenance 44  
Remote control 39
- S**  
Safety regulations 6  
Service 44  
Servicing 44  
Setting parameters 26, 35  
Setting up 16, 18  
Setup 36  
Shelf 39  
Slide-in unit 39  
Storage after delivery 17  
Switching off 30  
Switching on 22

**T**

TB 30  
Technical data 13  
Temperature 27  
Temperature comparison 42  
Temperature deviation 42  
Temperature limiter 30  
Temperature monitoring 28,  
37  
Time 39  
Timer 27  
Timer mode 39  
Transport 16, 17  
Transport damage 17  
Turn control 26  
TWB 28  
TWW 28

**U**

Unit 37  
Unpacking 17

**W**

Warning messages 12, 31  
Weight 13



# memmert

Experts in Thermostatics

Universal ovens

Incubators

D33363 | Date 06/2016

englisch

Memmert GmbH + Co. KG  
Willi-Memmert-Straße 90-96 | D-91186 Büchenbach  
Tel. +49 9122 925-0 | Fax +49 9122 14585  
E-Mail: [sales@memmert.com](mailto:sales@memmert.com)  
[facebook.com/memmert.family](https://facebook.com/memmert.family)  
Die Experten-Plattform: [www.atmosafe.net](http://www.atmosafe.net)